

3M™ PICC/CVC Securement Device

Product Description

3M™ PICC/CVC Securement Device is used to secure Peripherally Inserted Central Catheters (PICCs) and short term Central Venous Catheters (CVCs) to the skin.

The molded plastic device is integrated onto a breathable base with a gentle silicone adhesive.

Indications for Use

3M™ PICC/CVC Securement Device is used to secure Peripherally Inserted Central Catheters (PICCs) and Short Term Central Venous Catheters (CVCs) to the skin. The device will accommodate the majority of single, double and triple lumen CVC catheters up to and including 12 French.

Warnings

- Do not use 3M™ PICC/CVC Securement Device where loss of adhesion could occur, such as with a confused patient, diaphoretic or non-adherent skin, or when the access device is not monitored daily.
- Failure to follow the manufacturer's instructions for use may result in complications including inadequate securement and skin irritation.
- This is a single use securement device. Reuse and/or repackaging may create a risk of patient or user infection, compromise the structural integrity and/or essential material and design characteristics of the securement device, which may lead to device failure.
- This securement device is intended to be used with a securement dressing.

Precautions

- Observe universal blood and body fluid precautions and infection control procedures, during application and removal of the securement device.
- Any active bleeding at the insertion site should be stabilized before applying the securement device.
- The skin should be dry and free of detergent residue to prevent skin irritation and to ensure good adhesion. Allow all preps and protectants to dry completely before applying the securement device.
- Do not use on patients with known tape or adhesive allergies.
- Avoid securement device contact with alcohol or acetone: both can weaken bonding of components and device adherence.
- Minimize catheter manipulation during application and removal of the securement device.
- Orient the device so arrows point toward the catheter insertion site.
- Securement device and catheter position should be routinely inspected.
- Securement device should be replaced at least every 7 days.
- Do not re-sterilize.

Directions for Use

Failure to follow the manufacturer's instructions for use may result in complications including inadequate securement and skin irritation.

3M™ PICC/CVC Securement Device: The device will accommodate the majority of single, double and triple lumen PICC and CVC catheters up to and including 12 French.

Site Preparation: Prepare the site according to institution protocol. Clipping of hair where the device and dressing will be placed may improve adhesion. Shaving is not recommended. The skin should be clean, dry and free of detergent residue. Allow all preps and skin protectants to dry completely before applying the securement device to prevent skin irritation and to ensure good adhesion.


Any active bleeding at the insertion site should be stabilized before applying the securement device.

Securement Device Application:

Minimize catheter manipulation during application of the 3M™ PICC/CVC Securement Device.

Refer to Figure 1 for device application instructions.

1. Before placing device on the skin, orient the device with arrows pointing toward the insertion site as shown in **Figure 1a**.
2. Place single, double or triple lumen CVC catheter into device as shown in **Figure 1b** and weave lumen(s) under the single plastic arm.
3. Remove liner of attached tape strip and secure lumen(s) to the device base as shown in **Figure 1c**.
4. Position device on skin at the desired location. Pull and remove liner from one side of base to expose adhesive while holding the device in place. Pull and remove liner from the other side of base.
5. Apply pressure to the device base to establish good adhesion to the skin.
6. Apply a securement dressing, such as the Tegaderm™ I.V. Advanced Securement Dressing (catalog number 1837 and 1839) or the Tegaderm™ CHG Chlorhexidine Gluconate I.V. Dressing (catalog number 1877 and 1879), following the manufacturer's instructions for use.

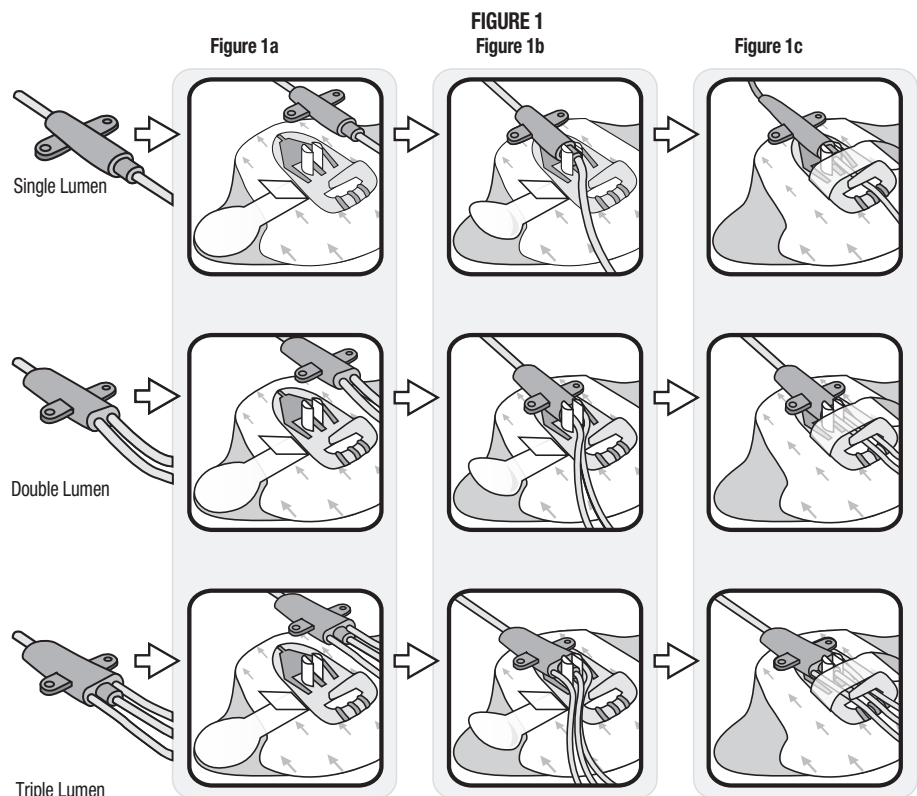

Site Care:

1. The site should be observed daily for signs of infection or other complications. If infection is suspected, remove the transparent dressing, inspect the site directly, and determine appropriate medical intervention. Infection may be signaled by fever, pain, redness, swelling, or unusual odor or discharge.
2. Inspect the securement device daily and change as necessary, in accordance with facility protocol. Securement device changes should occur at least every 7 days and may be needed more frequently with highly exudative sites or if integrity of the dressing is compromised.

Removal of Securement Device

Minimize catheter manipulation during removal of the 3M™ PICC/CVC Securement Device.

1. Using a low and slow technique, remove dressing in the direction of the catheter insertion site.
2. As the securement device is exposed secure the catheter hub with your gloved finger until device is uncovered. Leave remainder of dressing in place over catheter insertion site. **Figure 2**
3. Remove device tape strip from catheter lumen(s). **Figure 3**
4. Use gloved finger to stabilize the catheter hub and gently remove the catheter lumen(s) out from under the plastic arm of device.
5. Secure end of catheter lumens with tape to skin.
6. Stabilize catheter with one hand. Use your other hand to remove the device from skin and remove the remainder of dressing using a low and slow removal technique. **Figure 4**

Storage and Shelf Life

For best results, store in a cool, dry place. For shelf life, refer to the expiration date on the package.

Sterility of the device is guaranteed unless individual package is damaged or open.

How supplied / Ordering Information

For additional information visit www.3M.com









3M™ PICC/CVC Securement Device	
Catalog #	Device size
2100	2" x 2 1/8" (5.1 cm x 5.4 cm)

If you have any questions or comments, in the USA please contact the 3M Health Care Customer Help line at 1-800-228-3957.

In Canada, contact 3M Canada Company, P.O. Box/C.P. 5757, London, Ontario, N6A 4T1, 1-800-364-3577.

For further information outside the United States, contact your local 3M representative or contact us at 3M.com and select your country.

Explanation of Symbols

-  Do not use if package is damaged or open
-  This product and package do not contain natural rubber latex.
-  Caution, see instructions for use
-  Do not reuse
-  Use by date
-  Batch code
-  Manufacturer
-  Sterilized using ethylene oxide

-  Do not resterilize

3M Health Care

2510 Conway Ave.
St. Paul, MN 55144 U.S.A.
1-800-228-3957
3M.com/C3SD

3M is a trademark of 3M.
Used under license in Canada.
© 2013, 3M. All rights reserved.

Issue Date: 2013-11
34-8713-7969-8

3M Canada Company
C.P. Box 5757
London, Ontario, N6A 4T1
1-800-364-3577
3M.com/C3SD

3M est une marque de commerce de 3M, utilisée sous licence au Canada.
© 2013, 3M. Tous droits réservés.




Figure 2




Figure 3




Figure 4