
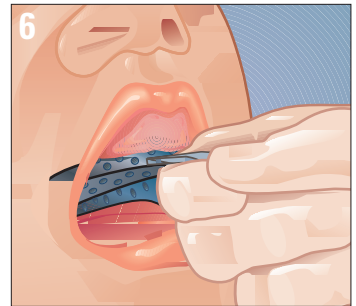
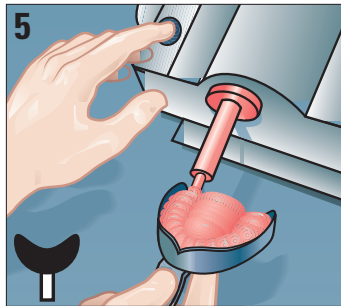
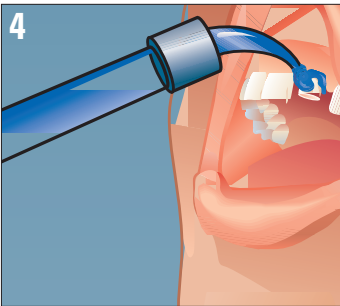
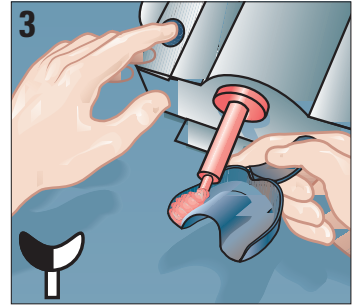
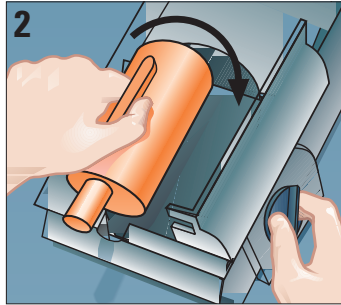


Permadyne® Penta L – Step-by-step

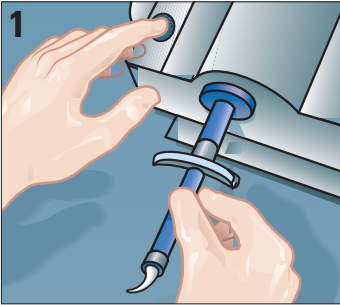


Permadyne Penta L

Permadyne Penta H

min:sec

min:sec

0:15




0:15

0:30

1:00

Start Syringing

max
2:15



3:15

6:30



0:15

0:15

0:30

0:30


1:00

0:30

Seat Tray

3:15

3:15 Setting Time



6:30