



Science.
Applied to Life.™



Your source for accurate impressions

Technique Guide for Clear Aligner Impressions

A perfect balance puts you in control

Imprint™ 4 VPS Impression Material helps you optimize your impression procedure with innovative chemistry that lets you save time AND get accurate results.



Speed

Fast setting time for your patients.

Choosing a fast-setting impression material minimizes the time the impression is in the mouth—this reduces stress for patients, and reduces the possibility of errors.

Imprint 4 VPS Impression Material offers the fastest intra-oral setting time among leading VPS fast-setting impression materials,¹ offering a real time savings. How?

The innovative active self-warming feature accelerates setting time.

Once in the mouth, the material warms up to body temperature (37°C/98.6°F). This speeds up the setting reaction which results in a short intra-oral setting time.

Control

Long working time for you.

Having adequate working time is important for accurate results. Imprint 4 material gives you all the working time you need.

Due to the unique chemistry, the setting time doesn't start until the END of the working time. That means you'll have a sufficient amount of time to load and seat the tray—no stressful race against the clock.

Whether you use a 1-step or 2-step impressioning technique, Imprint 4 material puts you in control of your everyday crown and bridge cases.

Precision

Super hydrophilicity.

Imprint 4 material is super-hydrophilic, and displaces moisture right from the start in the unset state. That allows the material to reproduce accurate details even in a moist environment—giving you ultimate precision and confidence. Choose it for:

- impressions with precise details that are easy to read, and
- precise-fitting restorations

Summary of Advantages

- Shortest intra-oral setting time for real time savings
- Sufficient working time for a stress-free procedure
- Super hydrophilicity for accurate detail reproduction, even in a moist environment
- Clinically proven tear strength
- Fresh material colors for easier readability
- Patient-pleasing mint flavor

Clinical step-by-step technique for clear aligner impressions

Prepare materials, equipment and review technique guidelines before beginning procedure. Try in impression trays to ensure proper fit.

Guidelines for G

Impression Trays

Before taking an impression, try-in the tray for proper fit. No teeth or support tissue should hit the tray during the try-in. Use proper tray size for the patient's arch. Extra large, large, medium and small trays are available. For Invisalign® cases, you must use only Invisalign branded impression trays. Trays can be altered or manipulated by using a torch to warm the plastic. You can also use a lab acrylic bur to adjust tray margins for patients who have large torri.

Maxillary Impression Steps



1. Load impression tray with Imprint™ 4 Penta Putty starting with posterior of impression.



2. Load the impression tray while keeping the tip immersed in material to avoid air bubbles and voids. **NOTE: 1:30 working time with Imprint™ 4 Penta Putty.**



3. Using your index finger, make a trough in the putty where the maxillary teeth will be. Be sure to allow room for light body wash in the trough.




4. Pinch the putty to extend the material in the vestibule area.



5. Examine the putty in the tray to make sure you have good depth for the Imprint™ 4 Light Body Wash Material.



6. Dispense Imprint™ 4 Light Body Wash Material into the trough, making sure to keep the tip immersed in the material while dispensing.

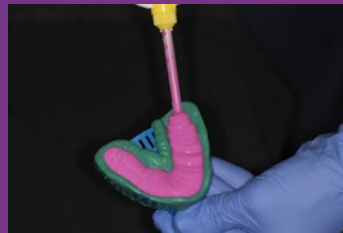


7. Apply an even amount of Imprint™ 4 Light Body Material in order to get a good detailed impression. **NOTE: 1:00 working time with Imprint™ 4 Light Body.**



8. Seat the impression straight up to avoid any drags or scrapes. Make sure the handle is always aligned up with the patient's midline.



9. Always hold the impression tray in the pre-molar area for stability. **NOTE: 2:30 intra-oral set time. Keep in patient's mouth 2:30.**

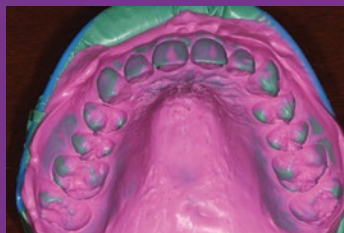

10. Final maxillary impression with Imprint™ 4 Penta Putty and Imprint™ 4 Light Body Wash Material. Disinfect the impression and package for shipment for aligner fabrication.

Note: To complete this impression technique with a Heavy Body/ Light Body material combination (instead of putty material), complete steps 1, 2 and 6 – 10. Instead of dispensing Light Body material into the trough of the impression (steps 6 and 7) you'll dispense Light Body material across the top of the Heavy Body material.

ood Impressions

Impression Material

Use only VPS/PVS materials — do not use polyether, alginate or alginate alternative materials. Cases submitted do require both an upper and lower impression. It is important to remember that impressions will not be returned. If needed, take a second set of impressions for your records.

Expiration Date and Temperature

Always check the expiration date on both tray and injected impression materials. Expired impression material may not set properly. Impression materials must be stored at room temperature (73°F). Storing at lower temperatures will prolong setting times and storing at an elevated temperature will reduce setting times.

Inadequate Mix

After removing the impression material cartridge cap, extrude or bleed the material before applying mix tip. This will ensure even flow for dispensing material. Do not substitute mixing tips. Always use the supplied manufacturer mixing tips and follow instructions for use.

Follow Manufacturers Directions

Ensure mix tip is correctly attached. Impression tips are different in size and color. Check the manufacturer's directions for which tip should be used. When using a putty or hand-mix impression material, always use the supplied measuring scoop to ensure proper ratios of material.

Mandibular Impression Steps



1. Load impression tray with Imprint™ 4 Penta Putty starting with posterior of impression.



2. Load the impression tray while keeping the tip immersed in material to avoid air bubbles and voids. **NOTE: 1:30 working time with Imprint™ 4 Penta Putty.**




3. Using your index finger, make a trough in the putty where the maxillary teeth will be. Be sure to allow room for light body wash in the trough.



4. Pinch the putty to extend the material in the vestibule area.



5. Dispense Imprint™ 4 Light Body Wash Material into the trough, making sure to keep the tip immersed in the material while dispensing.

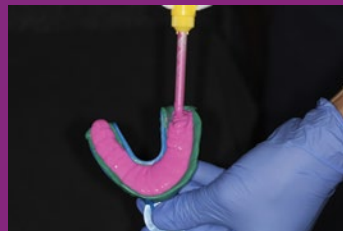

6. Apply an even amount of Imprint™ 4 Light Body Material in order to get a good detailed impression. **NOTE: 1:00 working time with Imprint 4 Light Body.**



7. Seat the impression straight down over arch while pulling out the patient's cheek.



8. Move around behind the patient holding down the impression in the pre-molar area with thumbs for stability while gently holding the mandible with fingers. **NOTE: 2:30 intra-oral set time. Keep in patient's mouth 2:30.**



9. Final maxillary impression with Imprint™ 4 Penta Putty and Imprint™ 4 Light Body. Disinfect the impression and package for shipment for aligner fabrication.

NEVER ask the patient to hold tray
ask the patient to bite together
have the patient bite on cotton rolls

Tips for success

Insert the tray straight up. Once the tray is stabilized after seating, avoid any movements. Patients should close their mouth as much as possible without biting down on the tray to avoid deformation of the mandible and, thus, errors in the impression. Do not try to correct the position of the tray after insertion.

3M's Imprint™ 4 VPS Impression Material has the fastest intra-oral setting time which means less time for unintended movements.



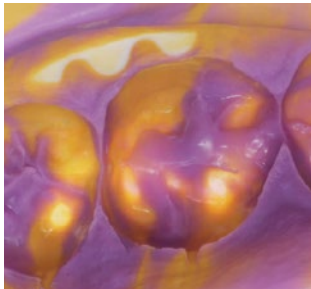



Upper jaw impression.



Lower jaw impression.

Impression troubleshooting

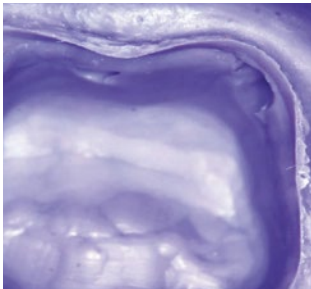Problem				
	Voids on the margin	Facial-oral flow defects	Show-through of tray	Poor bond between tray and wash material
Causes	<ul style="list-style-type: none"> • Air trapped in Intra-Oral Syringe • Air trapped while filling impression tray 	<ul style="list-style-type: none"> • Exceeding working time • Tray movement after initial seating • Tray doesn't support flow of material 	<ul style="list-style-type: none"> • Tooth contact on sides or bottom of impression tray • Insufficient amount of material utilized • Missing dentition in posterior 	<ul style="list-style-type: none"> • Exceeding working time • Improper mix of material • Impression material was not bled prior to use
Solutions	<ul style="list-style-type: none"> • Properly bleed filled syringe • Keep mixing tip immersed in material when filling • Use adequate material 	<ul style="list-style-type: none"> • Follow manufacturer guidelines for working/setting time • Don't move tray following seating • Use proper tray selection 	<ul style="list-style-type: none"> • Identify correct tray size prior to taking impression • Use sufficient material • Check tray length prior to impression 	<ul style="list-style-type: none"> • Follow manufacturer suggested working/setting times • Use correct mix tips • Always bleed a small amount of material before starting

Ordering Information

Item #	Product Information
Intro Kits	
71494	Imprint™ 4 Penta™ Heavy Intro Kit Kit includes: 1 – 300ml base paste; 1 – 60ml catalyst; 1 – 50ml Light cartridge; 1 – 50ml Regular cartridge; 1 – Penta™ cartridge; 10 – Penta™ mixing tips, red; 5 – 3M™ ESPE™ Intra-Oral Syringes, green; 5 – mixing tips, yellow; 5 – intra-oral tips, yellow; 1 – VPS tray adhesive
71495	Imprint™ 4 Penta™ Super Quick Heavy Intro Kit Kit includes: 1 – 300ml base paste; 1 – 60ml catalyst; 1 – 50ml Super Quick Light cartridge; 1 – 50ml Super Quick Regular cartridge; 1 – Penta™ cartridge; 10 – Penta™ mixing tips, red; 5 – 3M™ ESPE™ Intra-Oral Syringes, green; 5 – mixing tips, yellow; 5 – intra-oral tips, yellow; 1 – VPS tray adhesive
71536	Imprint™ 4 Penta™ Putty Intro Kit Kit includes: 1 – 300ml base paste; 1 – 60ml catalyst; 1 – 50ml Super Quick Light cartridge; 1 – 50ml Regular cartridge; 1 – Penta™ cartridge; 10 – Penta™ mixing tips, red; 5 – 3M™ ESPE™ Intra-Oral Syringes, green; 5 – mixing tips, yellow; 5 – intra-oral tips, yellow; 1 – VPS tray adhesive
71534	Imprint™ 4 Intro Kit Kit includes: 2 – 50ml Heavy cartridges; 1 – 50ml Light cartridge; 1 – 50ml Regular cartridge; 10 – mixing tips, green; 10 – 3M™ ESPE™ Intra-Oral Syringes, green; 1 – VPS tray adhesive
71535	Imprint™ 4 Super Quick Intro Kit Kit includes: 2 – 50ml Super Quick Heavy cartridges; 1 – 50ml Super Quick Light cartridge; 1 – 50ml Super Quick Regular cartridge; 10 – mixing tips, green; 10 – 3M™ ESPE™ Intra-Oral Syringes, green; 1 – VPS tray adhesive
Penta™ Refills—Tray Materials Each refill includes: 2 – 300ml base pastes; 2 – 60ml catalysts	
71484	Imprint™ 4 Penta™ Heavy
71485	Imprint™ 4 Penta™ Super Quick Heavy
71486	Imprint™ 4 Penta™ Putty
Refills—Tray Materials Each refill includes: 4 – 50ml cartridges; 10 – mixing tips, green	
71492	Imprint™ 4 Heavy
71493	Imprint™ 4 Super Quick Heavy

Item #	Product Information
Economy Packs—Tray Materials Each Economy Pack includes: 10 – 50ml cartridges	
71531	Imprint™ 4 Heavy Economy Pack
71532	Imprint™ 4 Super Quick Heavy Economy Pack
Refills—Wash Materials Each refill includes: 4 – 50ml cartridges; 5 – mixing tips, yellow; 5 – 3M™ ESPE™ Intra-Oral Syringes, green	
71488	Imprint™ 4 Light
71487	Imprint™ 4 Regular
71490	Imprint™ 4 Super Quick Light
71489	Imprint™ 4 Super Quick Regular
Cartridges for Pentamix™ 3 Automatic Mixing Unit	
77784	Imprint™ 4 Heavy
77785	Imprint™ 4 Super Quick Heavy
77786	Imprint™ 4 Penta™ Putty
Cartridges for Pentamix™ 2 Automatic Mixing Unit	
77781	Imprint™ 4 Heavy
77782	Imprint™ 4 Super Quick Heavy
77783	Imprint™ 4 Penta™ Putty
Accessories	
77949	Penta™ Mixing Tips – Red (50 – mixing tips)
71452	Garant™ VPS Mixing Tips – Yellow (50 – mixing tips)
71462	Garant™ VPS Intra-Oral Mixing Tips – Yellow (50 – intra-oral tips)
71450	Garant™ VPS Mixing Tips – Green (50 – mixing tips)
71506	3M™ ESPE™ Intra-Oral Syringe – Green (50 – intra-oral syringes)

Make better impressions.

Nothing compares to a good first impression. Experience the superior results for your patients by selecting impressing materials from 3M ESPE Dental, the worldwide leader in impression materials.

The 3M Impression Trouble Shooting Guide identifies common problems and offers solutions. To get your FREE copy, download it now from our website — www.3MESPE.com/GreatImpressions.



Customer Care Center: 1-800-634-2249



3M Oral Care
2510 Conway Avenue
St. Paul, MN 55144-1000 USA

Phone 1-800-634-2249
Web 3M.com/Imprint4

3M Canada
Post Office Box 5757
London, Ontario N6A 4T1
Canada

Phone 1-888-363-3685

All images used with permission from Contemporary Product Solutions. Contemporary Product Solutions provides expertise in clinical and laboratory evaluation of dental products and equipment from the total team perspective.

3M, ESPE, Garant, Imprint, Penta and Pentamix are trademarks of 3M or 3M Deutschland GmbH. Used under license in Canada. All other trademarks or registered trademarks are the property of their respective owners.

Please recycle. Printed in U.S.A. © 3M 2015.
All rights reserved. 70-2013-0715-7