


Why one modality stands out from the rest for measuring patient core temperature.



Core body temperature is a critical vital sign that should be monitored throughout the perioperative journey

Proactively monitoring temperature with a consistent, accurate, and non-invasive system is the only true way to own the normothermic temperature zone (36.0°C - 37.5°C) and protect patients from unintended perioperative hypothermia.

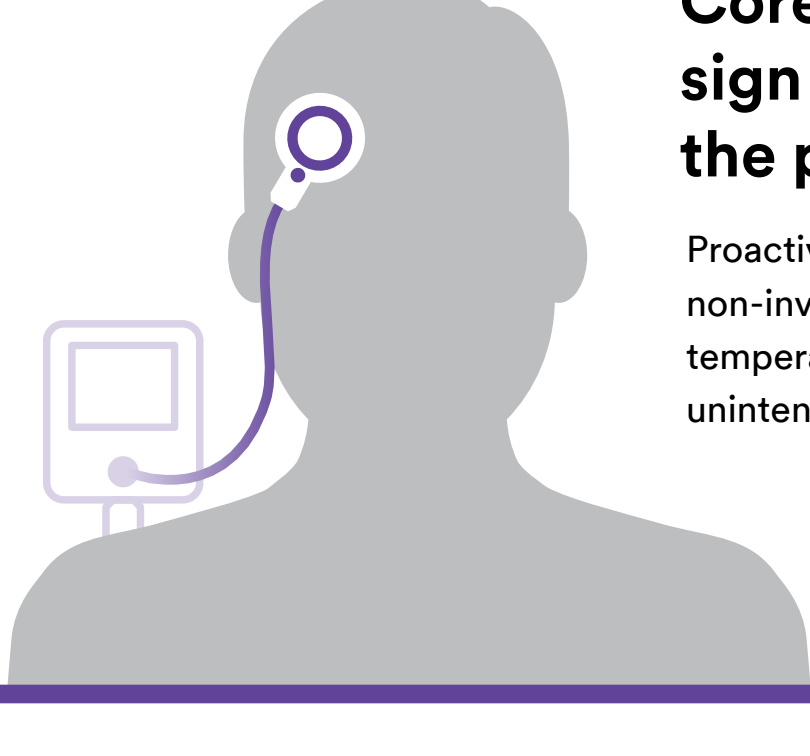

The importance of measuring and monitoring core temperature

Inadvertent perioperative hypothermia is defined as a core body temperature of less than 36.0°C, which can:

- Increase the rate of SSIs²** (Icon: Magnifying glass over bacteria)
- Increase surgical blood loss³** (Icon: Blood drop)
- Lead to increased mortality⁴** (Icon: ECG with heart)
- Extend recovery time⁵** (Icon: Clock)
- Cause patient discomfort⁶** (Icon: Patient in bed)


Inadequate monitoring of core temperature can increase the risk of death associated with malignant hyperthermia (MH).^{7, 8}

STAY AHEAD OF HYPOTHERMIA WITH A TEMPERATURE REVIEW

- 30%** When temperature was not monitored, 30% of patients with an MH episode died.^{7, 8}
- 2%** If core temperature monitoring was used, the risk of death was reduced to 2% (P = 0.0012).^{7, 8}

Temperature monitoring trade-offs

Most current technologies are unable to non-invasively and accurately measure core body temperature. The 3M™ Bair Hugger™ Temperature Monitoring System can do both, allowing you to improve active warming practices. You can only manage what you can accurately measure.

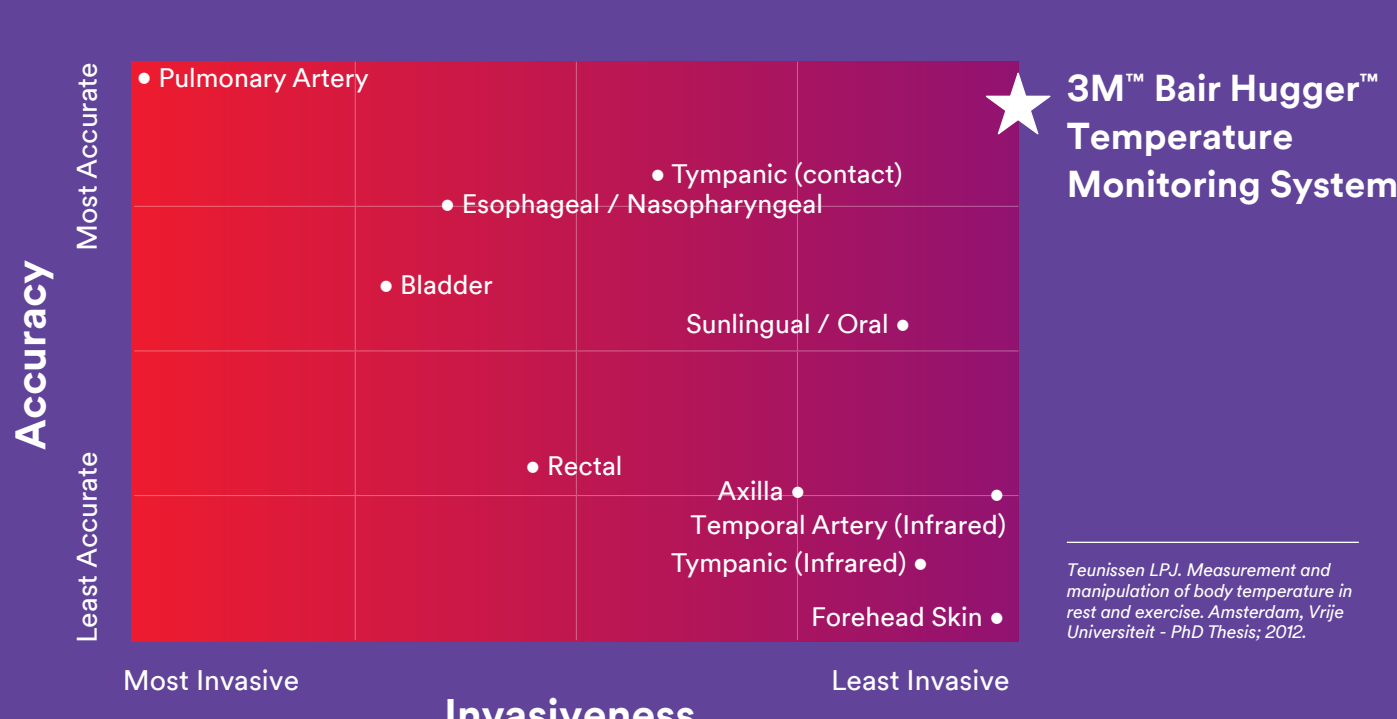

Global guidelines:

- AORN⁹** recognizes zero-heat-flux as a core temperature modality
- ASPAN¹⁰** recommends the use of one modality throughout the perioperative journey
- NICE¹¹** recommends continuous temperature monitoring
- DGAI¹²** recommends continuous core temperature monitoring with a consistent method


Download the Temperature Monitoring white paper to see how the Bair Hugger System compares to other modalities.

The future of non-invasive temperature monitoring is here


The Bair Hugger temperature monitoring system is the first accurate, non-invasive solution that allows you to easily monitor core body temperature consistently throughout the perioperative journey.

- Clinically equivalent to invasive methods¹³**
- Eliminates the potential of trauma from invasive modalities^{14, 15}**
- Displays current and 2-hour temperature trends**
- One modality eliminates variability**

Technology that's more than skin deep

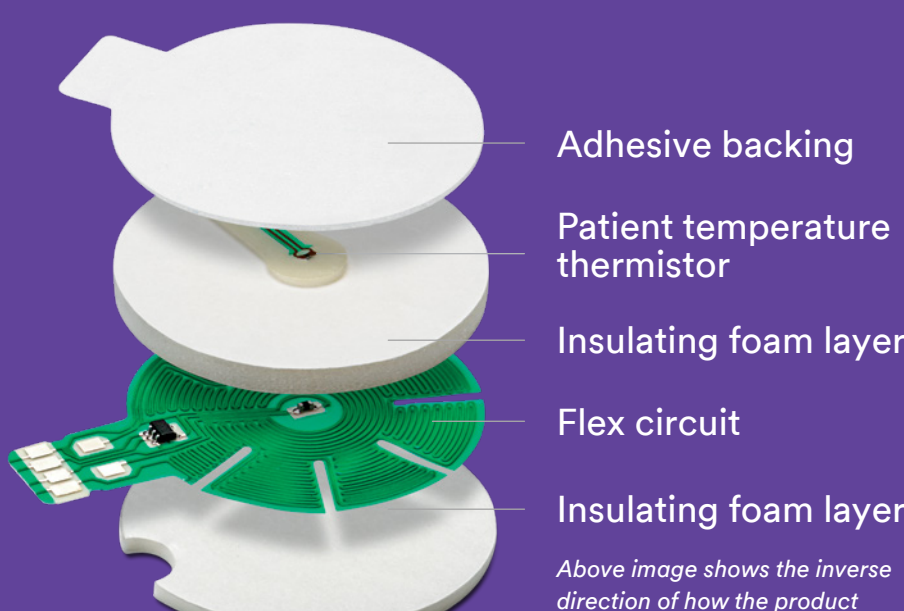


Zero-heat-flux technology produces near-perfect insulation, so heat cannot escape from the skin surface, creating an isothermal pathway.

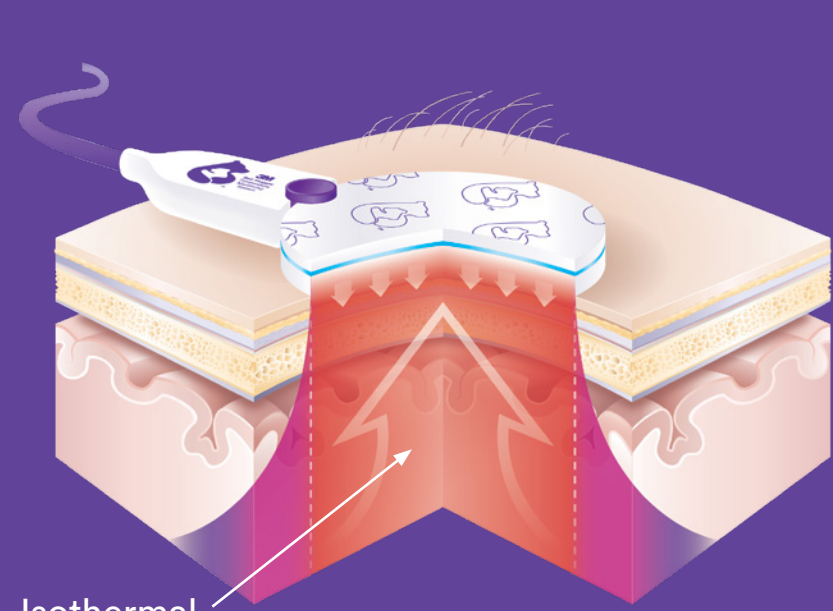

Monitor with confidence

The Bair Hugger temperature monitoring system makes it possible to get accurate readings throughout the entire perioperative journey with a single sensor.

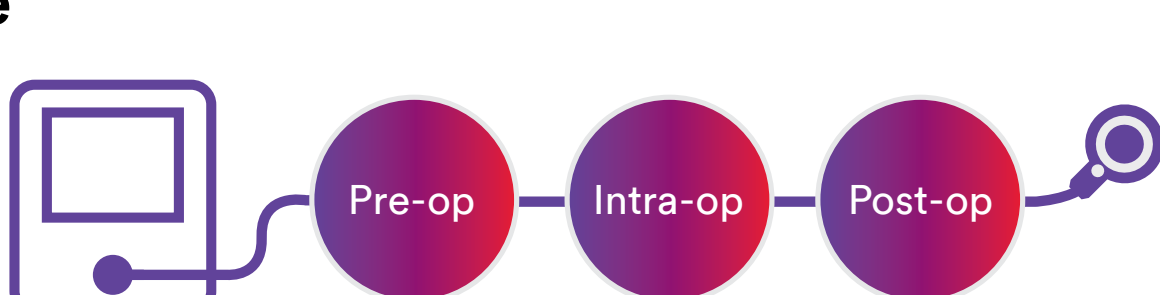

The sensor remains on the patient throughout the perioperative journey but may be disconnected from and reconnected to the control unit as needed.

EXPLORE THIS PROVEN SOLUTION

One sensor, one proven solution

Now that there is one accurate, consistent temperature monitoring solution, you have the power to Own the Zone.



Ready to own the zone? **CONTACT YOUR 3M SALES REPRESENTATIVE**

Fight SSIs from every angle.



3M, BAIR HUGGER and the BAIR HUGGER logo are registered trademarks of 3M. Please recycle. Printed in U.S.A. © 3M 2018. All rights reserved.

3M Health Care
2510 Conway Ave.
St. Paul, MN 55144 U.S.A.
800-228-3957 | www.bairhugger.com

70-2011-7099-3

1 Schroeck H, Lyden AK, Benedict WL, Ramachandran SK. Time Trends and Predictors of Abnormal Postoperative Body Temperature in Infants Transported to the Intensive Care Unit. *Anesthesiology Research and Practice*. 2016;7:18137.
2 Kurz A, Sessler DI, Lenhardt R. Perioperative normothermia to reduce the incidence of surgical-wound infection and shorten hospitalization. *NEJM*. 1996 May 9;334(19):1209-16. Melling AC, Ali B, Scott EM, Leaper DJ. Effects of preoperative warming on the incidence of wound infection after clean surgery: a randomised controlled trial. *The Lancet*. 2001 Sep 15;358(9265):876-80. Scott AV, Stonemetz JL, Wasey JO, Johnson DJ, Rivers RJ, Koch CG, et al. (2015) Compliance with Surgical Care Improvement Project for Body Temperature Management (SCIP Inf-10) Is Associated with Improved Clinical Outcomes. *Anesthesiology* 123: 116-125.
3 Schmied H, Reiter A, Kurz A, Sessler DI, Kozek S. Mild hypothermia increases blood loss and transfusion requirements during total hip arthroplasty. *The Lancet*. 1996 Feb 3;347(8997):289-92.
4 Bush H Jr, Hydo J, Fischer E, et al. Hypothermia during elective abdominal aortic aneurysm repair: The high price of avoidable morbidity. *J Vasc Surg*. 1995;21(3): 392-402.
5 Lenhardt R, Marker E, Goll V, et al. Mild intraoperative hypothermia prolongs postanesthetic recovery. *Anesth*. 1997;87:1318-23.
6 Sessler DI. Current Concepts: Mild perioperative hypothermia. *NEJM*. 1997. Vol. 336, No. 24, pp. 1730-1737.
7 Larach MG, Brandom BW, Allen GC, Gronert GA, Lehman EB. Malignant Hyperthermia Deaths Related to Inadequate Temperature Monitoring, 2007-2012: A Report from The North American Malignant Hyperthermia Registry of the Malignant Hyperthermia Association of the United States. *Anesthesia & Analgesia*. 2014;119(6):1359-1366.
8 Shafer SL, Dexter F, Bull SJ. Deadly Heat: Economics of Continuous Temperature Monitoring During General Anesthesia. *Anesthesia & Analgesia*. 2014;119(6):1235-1237.
9 Association of periOperative Registered Nurses.
10 American Society of PeriAnesthesia Nurses.
11 National Institute for Health and Care Excellence.
12 German Society of Anaesthesiology and Intensive Care Medicine.
13 <0.28°C error between Bair Hugger™ Temperature Monitor and a nasopharyngeal probe. <0.28°C error between Bair Hugger™ Temperature Monitor and a pulmonary artery catheter.
14 Insler SR, Sessler DI. Perioperative thermoregulation and temperature monitoring, 2006. *Anesthesiology Clinics*, (24): 823-837.
15 Cereda M, & Maccloli GA. Intraoperative temperature monitoring, 2004. *International Anesthesiology Clinics*, (42):2: 41-54.