

3M[™] V.A.C.[®] Ulta 4 Therapy Unit with 3M[™] V.A.C.[®] Therapy

V.A.C.[®] Ulta 4 Therapy Unit



Setting up the therapy unit


1. Attach the canister





V.A.C.® Therapy: 500ml or 1000ml canister (acute care only).


2. Connect the dressing tubing (after applying the dressing) Align, push, and twist





Note: Refer to the instructions for use for complete details regarding dressing application.

Initiating V.A.C.[®] Therapy

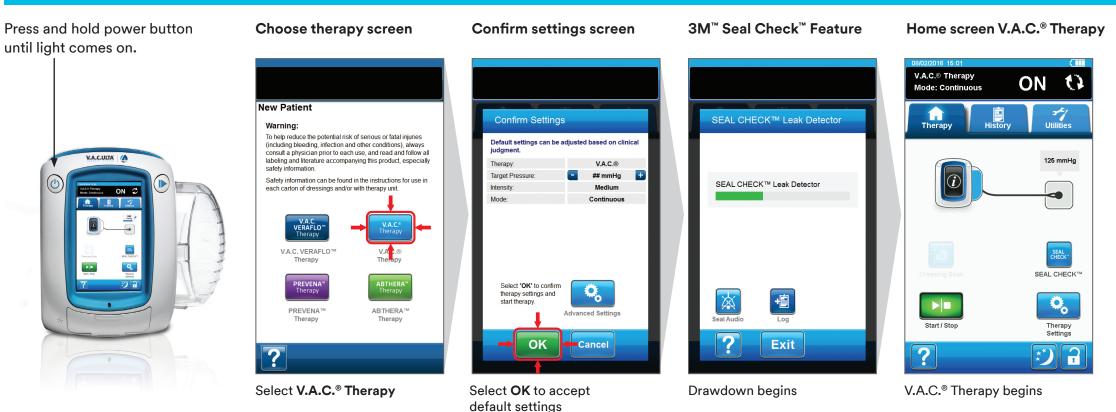

Enhanced features

Contraindications

Do not place foam dressings of the V.A.C.[®] Ulta Therapy System (including both V.A.C. Therapy and 3M[™] V.A.C. Veraflo[™] Therapy Dressings) directly in contact with exposed blood vessels, anastomotic sites, organs, or nerves.

Pre-leak indicator early detection system

V.A.C. Therapy Home screen.



The yellow box around the dressing notifies the user that a leak is present and an alarm will occur soon if not addressed.

3M[™] Dynamic Pressure Control[™] Therapy

V.A.C.[®] Therapy advanced settings screen.



Configure V.A.C Therapy as prescribed and select **OK**.

V.A.C.[®] Therapy is contraindicated for patients with:

- Malignancy in the wound.
- Untreated osteomyelitis.
- Non-enteric and unexplored fistulas.
- Necrotic tissue with eschar present (Note: After debridement of necrotic tissue and complete removal of eschar, V.A.C.® Therapy may be used.).
- Sensitivity to silver (3M[™] V.A.C.[®] Granufoam Silver[™] Dressing only)

Note: Refer to the warnings and precautions section of the safety information sheet for additional information including details on potential risks associated with bleeding and infection. For complete information on indications, contraindications, and other safety information please reference the user manual and safety information sheet.

Note: If an alarm condition cannot be resolved, contact a healthcare provider or local representative.

Note: Specific indications, contraindications, warnings, precautions and safety information exist for these products and therapies. Please consult a clinician and product instructions for use prior to application. This material is intended for healthcare professionals.

© 2021 3M. All rights reserved. 3M and the other marks shown are marks and/or registered marks. Unauthorized use prohibited. 70-2013-1106-8 PRA-PM-AT-00061 (09/21)



3M[™] V.A.C.[®] Ulta 4 Therapy Unit with 3M[™] Veraflo[™] Therapy

Setting up the therapy unit

1. Press and hold the power button until light comes on.



3. Extend the solution container hanger arm





5. Connect the dressing tubing (after applying the dressing) Align, push, and twist.



Connect the installation line and then the V.A.C. Therapy line. Note: Refer to the Instructions for Use for complete details regarding Dressing Application.

Initiating Veraflo Therapy

Start up screen

Confirm settings

Confirm Settings	;
Default settings are sup can be adjusted based of	
Therapy:	V.A.C
Fill Assist	
Start Phase:	
Instill Volume:	F
Soak Time:	- 10
V.A.C.® Therapy Time:	3
Target Pressure:	12
Intensity:	
V.A.C.@ Therapy Mode:	





4. Spike and hang the solution container bag/bottle





6. Attach the 500ml or 1000ml canister



2. Once the startup screen is visible, attach

Solution container arm

V.A.C.[®] Ulta 4 Therapy Unit



Power button

Contraindications

Do not place foam dressings of the V.A.C.® Ulta Therapy System (including both V.A.C. Therapy and V.A.C. Veraflo Therapy Dressings) directly in contact with exposed blood vessels, anastomotic sites, organs, or nerves.

V.A.C. Therapy and Veraflo Therapy are contraindicated for patients with:

- Malignancy in the wound.
- Untreated osteomyelitis.
- Non-enteric and unexplored fistulas.
- Necrotic tissue with eschar present (Note: After debridement of necrotic tissue and complete removal of eschar, V.A.C.® Therapy may be used.).
- Sensitivity to silver (3M[™] V.A.C.[®] Granufoam Silver[™] Dressing only).

Note: Refer to the warnings and precautions section of the safety information sheet for additional information including details on potential risks associated with bleeding and infection. For complete information on indications, contraindications, and other safety information please reference the user manual and safety information sheet.

Additional contraindications specific to Veraflo Therapy:

- Do not use V.A.C. Dressings with Octenisept[®], hydrogen peroxide or solutions that are alcohol-based or contain alcohol.
- Do not deliver fluids to the thoracic or abdominal cavity due to the potential risk to alter core body temperature and the potential for fluid retention within the cavity.
- Do not use Veraflo Therapy unless the wound has been thoroughly explored due to the potential for inadvertent instillation of topical wound solutions to adjacent body cavities.

Fill assist screen

Fill assist screen

- 1 500 mL


+











Select Veraflo Therapy.

Select OK to accept default settings.



EAL CHECK™ Leak Detector

ote: This may take up to 2:30 minute Preparing dressing seal to minimize

3M[™] Seal Check[™] Feature

Drawdown begins.



Select start/stop on the fill assist screen to begin delivering solution to the wound.



Stop fill assist by depressing

start/stop. Select OK when

satisfied with instillation volume.



Veraflo Therapy begins

Enhanced features

Veraflo Therapy – advanced settings overview (optional)

Confirm Settings	
Default settings are supp can be adjusted based or	
Therapy:	V.A.C. VERAFLO™
Fill Assist:	ON
Start Phase:	Instill
Instill Volume:	Fill Assist
Soak Time:	😑 🛛 ## minutes 🛨
V.A.C.® Therapy Time:	😑 🗰 hour 🛨
Target Pressure:	💼 ## mmHg 🛨
Intensity:	Medium
V.A.C.® Therapy Mode:	Continuous
Select 'OK' to confirm therapy settings and start therapy.	Quanced Settings
ОК	Cancel

Select advanced settings.



Adjust pressure, intensity and therapy mode. Select OK to accept settings.



Turn fill assist off, select start phase. Adjust instill volume, soak time and V.A.C.[®] Therapy time.

Information screens – Veraflo Therapy

25/12/2016 12:00 V.A.C. VERAFLO ^{1M} Therapy Phase: DPC	ON ¢
Therapy History	- Utilities
	200 mmbig
Dressing Soak	SEAL CHECK
Start / Stop Pause / Resume	Co. Therapy Settings

Select i button from the home screen to continue to the therapy summary tab.

Therapy Summary	Current Settings	
Therapy Start Date:	****	
	Total	24hr
Total Therapy Time:	##:##:##	##:##:##
V.A.C.® Time:	##:##:##	##:##:##
Soak Time:	##:##:##	##:##:##
Therapy Cycles:	###	##
Instilled Volume:	### mL	## mL
Canister Last Changed:	##!##!## ##:##	
Cassette Last Changed:	##/##/## ##:##	
Dressing Last Changed:	##!##!## ##:##	
Solution Last Changed:	##/##/#	# ##:##
Reset 24hr Totals	Last: ##/##/#	
Ex	it	

Use the therapy summary tab to review a cumulative summary of therapy provided.

Therapy Summary	Current Settings
Therapy:	V.A.C. VERAFLO ***
Instill Volume:	## mL
Soak Time:	## minutes
V.A.C.® Therapy Time:	## hours
Target Pressure:	## mmHg
Intensity:	Medium
V.A.C.® Therapy Mode:	Continuous
Cycle Rise Time:	
Cycle Fall Time:	
Change	Settings

Use current settings tab to review the current therapy settings. Select change settings to continue to the confirm settings screen.

Note: If an alarm condition cannot be resolved, contact a healthcare provider or local representative.

Note: Specific indications, contraindications, warnings, precautions and safety information exist for these products and therapies. Please consult a clinician and product instructions for use prior to application. This material is intended for healthcare professionals.

© 2021 3M. All rights reserved. 3M and the other marks shown are marks and/or registered marks. Unauthorized use prohibited. 70-2013-1106-8 PRA-PM-AT-00061 (10/21)