

3M Infection Prevention
Cardiothoracic & Vascular Temperature Management



Cardiothoracic & Vascular Surgery

Temperature Management Strategies

Warming patients who are undergoing complex surgical procedures should not be complicated. 3M™ Bair Hugger™ therapy offers a number of easy to use blanket designs to actively warm—and rewarm—your most challenging cases, from pediatric to geriatric, without compromising surgical access.

3M Infection Prevention Solutions

Innovation
On A Mission

3M

3M™ Bair Hugger™ Therapy

Access From the Start

3M™ Bair Hugger™ therapy offers multiple warming solutions for cardiothoracic and vascular surgeries in pediatric and adult patient populations.

Underbody series blankets are placed on the OR table prior to the patient's arrival. This allows the care provider to focus on the patient and warm from the start of the procedure. As little as 15 minutes of forced-air warming prior to induction can add to the total heat content of the body helping to reduce the effects of redistribution temperature drop^{1,2} for procedures using a normothermic temperature management strategy.

The pediatric underbody blanket (model 555) and the large pediatric/small adult underbody blanket (model 550) offer excellent warming solutions for smaller patients. The full access underbody blanket (model 635) is ideally suited for the adult cardiothoracic or vascular surgery patient where unrestricted patient access is a requirement.

Temperature Management for Cardiothoracic and Vascular Surgery

Bair Hugger underbody series blankets will accommodate supine, lateral or prone positions and are suitable for use with either endovascular or open SVG harvesting techniques. Because the full access underbody blanket is in place under the surgical drapes, forced-air warming can be used to complement cardiopulmonary bypass rewarming strategies. The same blanket can be used to continue warming therapy after the patient has been weaned from bypass.

The full access underbody series blanket has been demonstrated to be more effective than a water mattress.^{2,3} Forced-air warming can also be used without the risk of thermal injury associated with conductive warming devices as a result of the combination of pressure, time and heat.⁴ Unlike with water mattresses, the patient's natural pressure points compress the forced-air underbody blanket preventing heat from reaching potentially ischemic tissue – areas that

Warm every patient

are at risk for pressure sore formation and thermal injury. All Bair Hugger underbody series blankets include unique drain holes that allow excess fluids to pass through the surface of the blanket to the linen below, reducing the potential for skin maceration or breakdown or inadvertent cooling⁵ of the surgical patient due to evaporative heat loss.


Bair Hugger temperature management units can be used to both actively warm or cool patients. In hypothermic bypass, the ambient setting may be used to complement CPB patient cooling while the medium and high settings can be used to complement

CPB patient rewarming.

Maintaining normothermia with forced-air warming has been shown to reduce the rate of complications such as:⁶

- Surgical site infection rates
- Post operative cardiac events
- ICU time
- Length of hospital stay
- Mortality rates
- Coagulopathy and transfusion of blood product
- Mechanical ventilation time

Temperature Management in Hypothermic Cardiac Surgery⁷

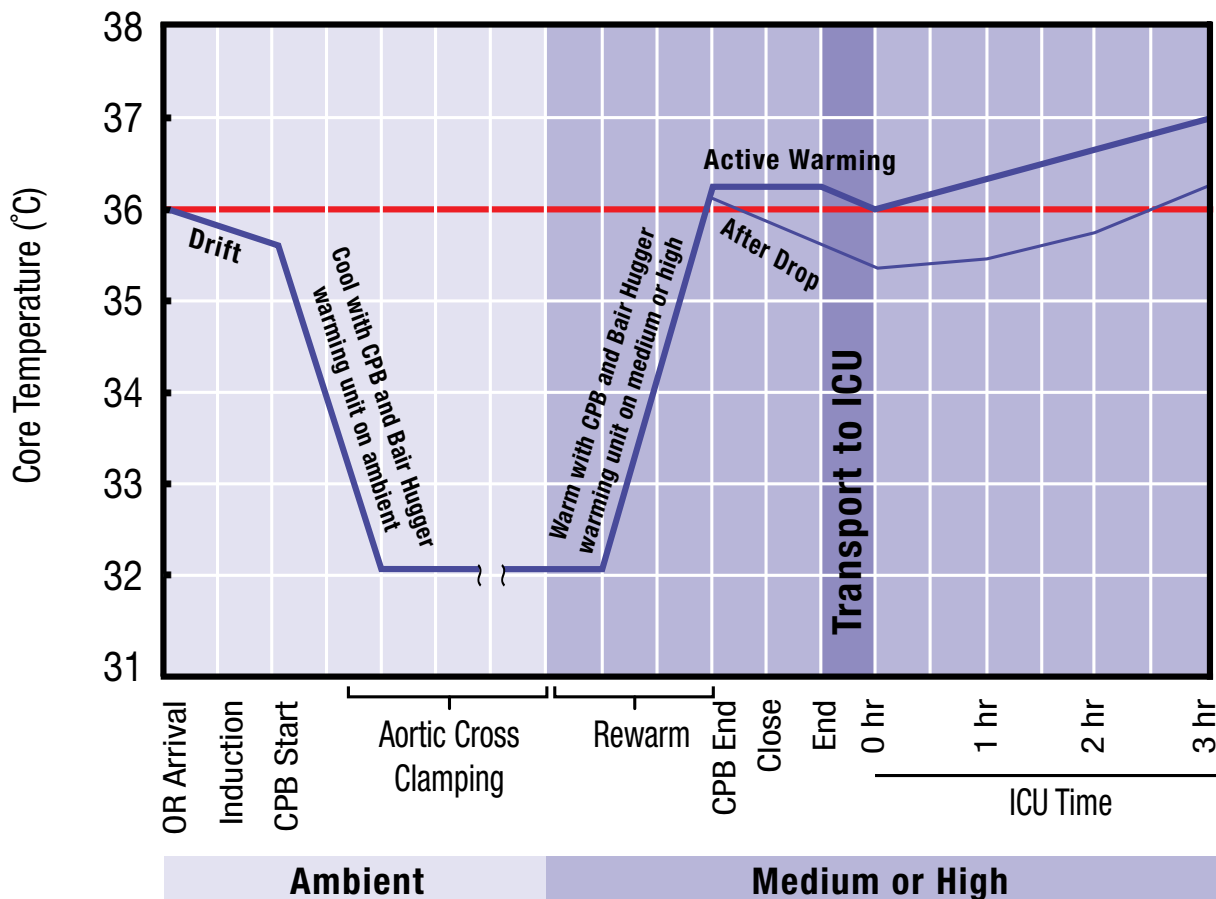

Adapted from: Hohn L, et al. Benefits of intraoperative skin surface warming in cardiac surgical patients. *British Journal of Anaesthesia*. 1998; 80(3): 318-323.



Pediatric Underbody
Model 555



Large Pediatric Underbody
Model 550



Sterile Cardiac
Model 630




Full Access Underbody
Model 635



Cummberrbund design allows for placement onto patient after surgical preparation.

External warming methods following hypothermic bypass⁸

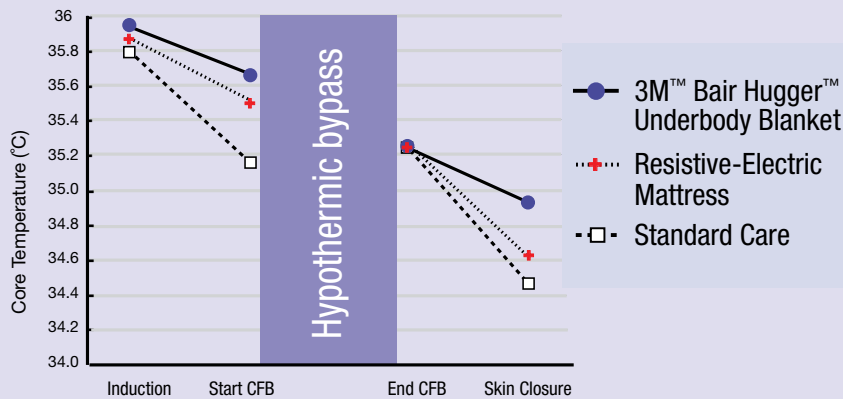

Adapted from: Engelen S., et. al. A Comparison of Under-Body Forced-Air and Resistive Heating During Hypothermic Bypass. *ASA Abstract*, 2010. A075.

On- and Off-Pump

Both on-pump and off-pump cardiothoracic and vascular procedures have demanding temperature management requirements.

Whether your surgical strategy involves near normothermic bypass or CPB-induced hypothermia where reducing the severity of post-bypass after drop is of concern, Bair Hugger therapy has demonstrated, flexible temperature management solutions designed to help you meet your patient temperature goals.


Bair Hugger underbody series blankets:

- Are significantly more effective at reducing unintended hypothermia following hypothermic CABG than resistive-electric type mattresses.⁸
- Are effective at preventing hypothermia and the harmful effects of hypothermia in the early postoperative phase in patients undergoing near-normothermic CABG.⁹
- Have been adopted for use in fast-track cardiac surgery to ensure a core temperature of 36°C.¹⁰


Studies have demonstrated that convective Bair Hugger underbody forced-air warming blankets produce superior intraoperative warming results when compared to conductive under-the-patient water mattresses^{1,5,11} or resistive-electric type heating mattress pads.⁸




INTRAOPERATIVE BLANKETS

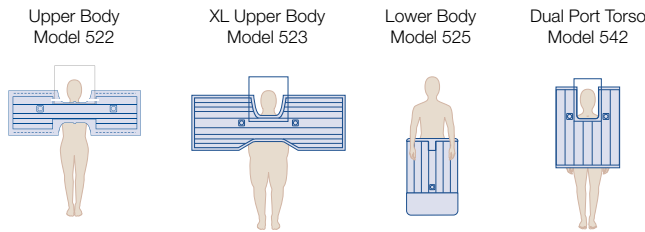


POSTOPERATIVE BLANKETS

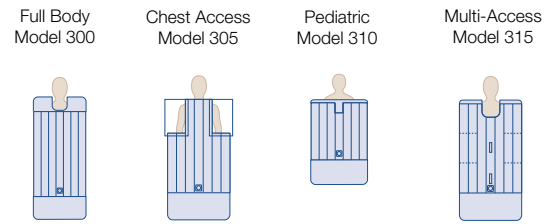

PEDIATRIC BLANKETS*




UNDERBODY SERIES

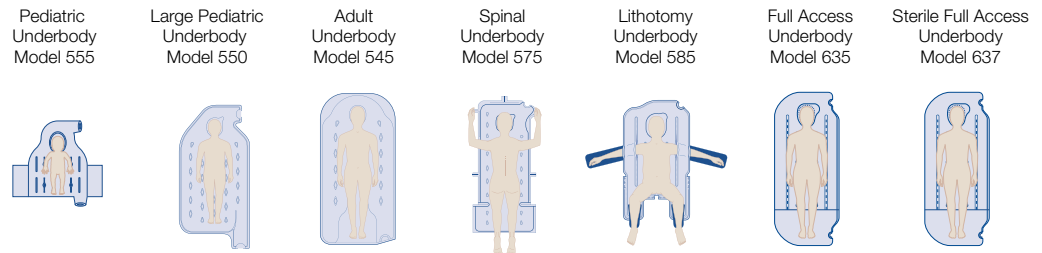

*Also see Underbody Series & PACU blankets

SPECIALTY AND CARDIAC BLANKETS

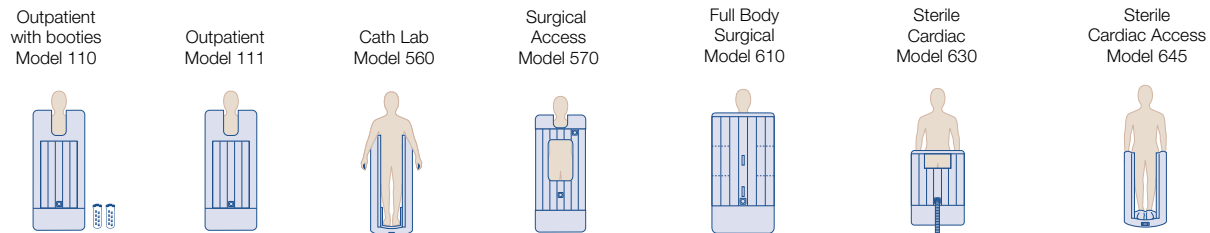

References:

- Sessler DI. Current concepts: mild perioperative hypothermia. *N Eng J Med*, 1997; 336: 1730-1737.
- Tominaga A, et. al. Efficacy of an Underbody Forced-Air Warming Blanket for the Prevention of Intraoperative Hypothermia. *Anesthesiology*, 2007; 107: A91.
- Ouchi T, et. al. Lithotomy Air Blanket can Prevent Intraoperative Redistribution Hypothermia. *ASA Abstract*, 2010; A088.
- Kokate JY, et. al. Temperature-modulated pressure ulcers: a porcine model. *Arch Phys Med Rehabil*, 1995; 76: 666-73.
- Lin EP. Wet forced air blankets are ineffective at maintaining normothermia. *Paediatric Anesthesia*, 2008; Jul;18(7):642-4.
- Mahoney CB. Odom J. Maintaining intraoperative normothermia: A meta-analysis of outcomes with costs. *AANA Journal*, 1999; 67(2): 155-164.
- Hohn L, et. al. Benefits of intraoperative skin surface warming in cardiac surgical patients. *British Journal of Anaesthesia*, 1998; 80: 318-323.
- Engelen S, et. al. A Comparison of Under-Body Forced-Air and Resistive Heating during Hypothermic Bypass. *ASA Abstract*, 2010; A075.
- Teodorczyk JE, et. al. Effectiveness of an Underbody Forced-Air Blanket in Preventing Postoperative Hypothermia after Coronary Artery Bypass Graft Surgery with Normothermic Cardiopulmonary Bypass. *Critical Care*, 2009; 13 (Suppl 1):P71.
- Ender J, et. al. Cardiac Surgery Fast-track Treatment in a Post-anesthetic Care Unit: Six-month Results of the Leipzig Fast-Track Concept. *Anesthesiology*, Jul 2008; No 1, V 109:61-6.
- Ong BC. A Prospective, Randomized and Controlled Clinical Trial using Parallel Design to Evaluate the Efficacy of Forced-Air Warming Bair Hugger Full Access Underbody Blanket in Maintaining Body Temperature as Compared to Circulating Water Warming Mattress and Forced-Air Warming Bair Hugger Cath Lab (U-Shape) Blanket in Coronary Artery Bypass Graft (CABG) Surgery. *SGH Proceedings*, 2009; Vol 18, No. 1 (Suppl):S39:1500.



Arizant Healthcare Inc.,
a 3M company
 10393 West 70th St.
 Eden Prairie, MN 55344 USA
 Phone 800-733-7775
 Fax 800-775-0002
 www.bairhugger.com

3M is a trademark of 3M Company, used under license in Canada. BAIR HUGGER and the BAIR HUGGER logo is trademarks of Arizant Healthcare Inc., used under license in Canada. ©2011 Arizant Healthcare Inc. All rights reserved. 603412A 9/11