



3M

Filtek™

**Supreme XTE
Universal Restorative**

Technical Product Profile

Table of Contents

Introduction	3
Product Description.....	4
Indications for Use	4
Composition	4
Shades	5
Fluorescence and Opalescence	6
Shade Basics.....	6
Colour.....	6
Opacity Considerations.....	7
Opinion Leaders.....	8
Shade Selection Tips and Hints for 3M™ Filtek™ Supreme XTE Universal Restorative.....	9
Shade Wheel.....	10
Background	12
Fillers.....	12
Microfills	12
Hybrids, Microhybrids and Nanohybrids	13
Nanocomposites.....	14
Filler Improvements in 3M™ Filtek™ Supreme XTE Universal Restorative	15
Resin System	16
<i>In Vitro</i> Handling Evaluations	16
Physical Properties	18
Polish Retention	18
Toothbrush Abrasion.....	18
Wyko Images.....	20
3-Body Wear	24
Fracture Toughness	25
Compressive and Diametral Tensile Strength.....	26
Flexural Strength and Modulus	28
Volumetric Shrinkage	30
Field Evaluation.....	31
Handling Acceptability	32
Questions and Answers.....	36
Endnotes.....	37
Technical Data Summary	38

Introduction

Building upon over 40 years of innovation in the field of restorative dentistry, at the turn of this century, 3M created a new category of dental material—the nanocomposite.

Through precise manipulation of the filler architecture at the nanoscale, 3M developed a breakthrough composite filling material, 3M™ Filtek™ Supreme Universal Restorative, that significantly advanced the clinical performance of universal composites. Up until the launch of this product, dentists desiring the highest aesthetics in direct composite restorations chose microfills. Microfills were considered the gold standard in aesthetics; however, their lack of strength, wear resistance and radiopacity limited their use to only select anterior restorations. Hybrid composites had high filler loading, but the average particle size was in the submicron range, which somewhat limited their aesthetic qualities. Hybrid composites provide the strength, wear resistance and radiopacity necessary for anterior and posterior use. In 2002, 3M launched Filtek Supreme restorative. This was the first product that utilised nanotechnology to provide the aesthetics of a microfill and the strength of a hybrid. All of the filler particles in this novel composite were engineered nanoparticles.¹ This technology provided lasting polish, excellent handling and wear similar to enamel.²

Subsequently, as a result of feedback from dentists, 3M™ Filtek™ Supreme XT Universal Restorative was launched in 2005. The shades were optimised to provide more vibrant, lifelike restorations as a result of increasing the value or brightness of the shades.

Since the original introduction of Filtek Supreme restorative, 3M has continued discussions with opinion leaders and general dentists regarding potential improvements desired. Based on these discussions, focus groups and other market research methods, additional improvements are realised with the introduction of 3M™ Filtek™ Supreme XTE Universal Restorative. The following improvements have been made to the system:

Easier-to-use shading system

- Colour coding by opacity
- New, easier-to-read labeling
- Extended Body shade range

Even better polish retention

Improved fluorescence

Supreme-like handling for all opacities

Improved Translucent shades

- Better Translucent shade handling
- Availability of Translucent shades in capsules
- Modified Translucent shade offering
- Translucent shades are radiopaque

Product Description

3M™ Filtek™ Supreme XTE Universal Restorative is a visible-light-activated composite designed for use in anterior and posterior restorations. All shades are radiopaque. A dental adhesive, such as those manufactured by 3M, is used to permanently bond the restoration to the tooth structure. The restorative is available in a wide variety of Dentine, Body, Enamel and Translucent shades. It is packaged in syringes and single-dose capsules.

Indications for Use

Filtek™ Supreme XTE restorative is indicated for use in:

- Direct anterior and posterior restorations (including occlusal surfaces)
- Core build-ups
- Splinting
- Indirect restorations (including inlays, onlays and veneers)

Composition

The resin system is slightly modified from the original 3M™ Filtek™ Z250 Universal Restorative and 3M™ Filtek™ Supreme Universal Restorative resin. The resin contains bis-GMA, UDMA, TEGDMA, and bis-EMA(6) resins. To moderate the shrinkage, PEGDMA has been substituted for a portion of the TEGDMA resin in 3M™ Filtek™ Supreme XTE Restorative.

The fillers are a combination of non-agglomerated/non-aggregated 20 nm silica filler, non-agglomerated/non-aggregated 4 to 11 nm zirconia filler, and aggregated zirconia/silica cluster filler (comprised of 20 nm silica and 4 to 11 nm zirconia particles). The Dentine, Enamel and Body (DEB)³ shades have an average cluster particle size of 0.6 to 10 microns. The Translucent (T)⁴ shades have an average cluster particle size of 0.6 to 20 microns. The inorganic filler loading is about 72.5% by weight (55.6% by volume) for the Translucent shades and 78.5% by weight (63.3% by volume) for all other shades.

Shades

The system is comprised of four opacities, listed here in decreasing order of opacity: Dentine (most opaque), Body, Enamel and then Translucent (very transparent). The opacity differences are illustrated in Figure 1. The clarity of the print under the 1 mm composite discs exhibits the opacity. The Translucent shades are very clear, hence the print appears relatively unchanged from the surrounding type. The Enamel shades have opacity similar to tooth enamel. The print is slightly fuzzy but very readable through the disc. The Body shades are slightly more opaque, less translucent than the Enamel shades to enable use in single-shade restorations. The print is still readable but very fuzzy. Dentine shades have the highest opacity. In multi-shade restorations, the Dentine shades are used to replace the more opaque Dentine tooth structure, alter underlying Dentine colour and block shine-through in anterior restorations.

The shade system is based on the VITA classical Shade Guide with the following exceptions:

- For bleached teeth: White Dentine, Body and Enamel (WD, WB, WE), Extra White Body and Enamel (XWB and XWE)
- For cervical restorations: A6B and B5B
- Translucent shades: Clear, Blue, Grey and Amber

The shade offering was modified from 3M™ Filtek™ Supreme XT Universal Restorative. The differences in the shade offering include a reduction in the Dentine shades (eliminated A6D, C6D, XWD). The Body shade offering was broadened by adding A6B and B5B for cervical restorations and D3B. An Enamel shade, XWE, was also added. Additionally, the Violet and Yellow Translucent shades were replaced with Blue and Amber Translucent.

The chart to the right also demonstrates the colour coding used in the 3M™ Filtek™ Supreme XTE Universal Restorative system. The darker the colour code, the more opaque the composite.

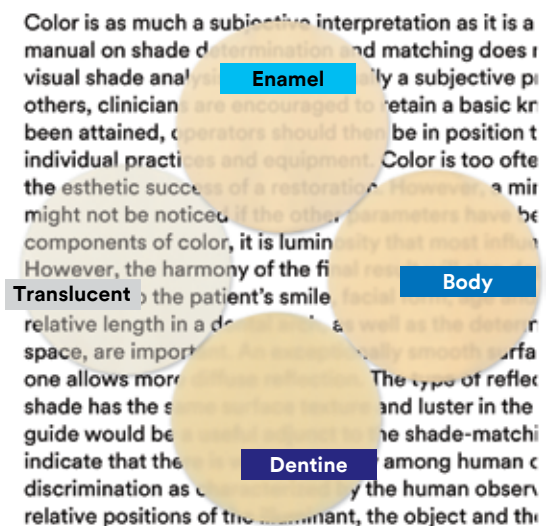


Figure 1: Opacity choices.

3M™ Filtek™ Supreme XTE Universal Restorative Shade Offering			
Dentine	Body	Enamel	Translucent
A1D	A1B	A1E	Clear
A2D	A2B	A2E	Blue
A3D	A3B	A3E	Grey
	A3.5B		Amber
A4D	A4B		
	A6B		
	B1B	B1E	
	B2B	B2E	
B3D	B3B		
	B5B		
	C1B		
	C2B		
	C3B		
C4D			
	D2B	D2E	
	D3B		
WD	WB	WE	
	XWB	XWE	

Fluorescence and Opalescence

Two additional aesthetic properties of natural dentition are fluorescence and opalescence. It is thought that both of these properties contribute to the vitality and lifelike appearance of dentition. In natural teeth, Dentine (more specifically the hydroxyapatite minerals and organic matrix) exhibits higher fluorescence than enamel. Fluorescence occurs when energy is absorbed and emitted at a longer wavelength. In teeth, this means the absorption of light in the UV region (350–365 nm) and emitting light in the visible region (~400 nm).⁵ As shown in Figures 2 and 3, teeth fluoresce blue-white. Note that some materials fluoresce more than the natural tooth, while others, e.g., 3M™ Filtek™ Supreme XTE Universal Restorative, fluoresce at a similar level and colour.⁶



Figure 2: Dentine, Enamel or Body shades.

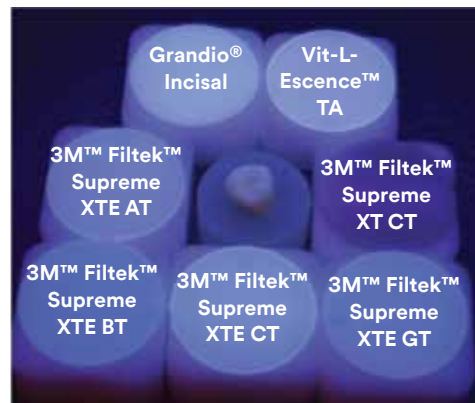


Figure 3: Translucent or Incisal shades.

Opalescence, on the other hand, is related to how a material scatters the shorter wavelengths of light. This is demonstrated by a bluish appearance under reflected light and orange/brown under transmitted light.⁷ Natural enamel exhibits an opalescent effect. By changing the nanocluster used, the Translucent shades of Filtek Supreme XTE restorative were specially formulated to provide the opalescence in the range of literature values for human enamel.⁸

Shade Basics

Colour

- Hue is the actual colour of the material. The bar below demonstrates the hues from blue to yellow.




- VITA classical Shade Guide Shade Family (Hue)

A shades	Red-brown character
B shades	Red-yellow character
C shades	Grey character (lower value)
D shades	Red-grey character (lower value)
- Chroma is the intensity of the shade. The higher the number (e.g., A3 vs. A1) within a shade family, the more intense the colour (A3 is more intense than A1).
- The value (amount of white or black) is higher (whiter) for the A and B shades. The C and D shades have lower value (greyer) than the A and B shades. Very generally speaking, the C shades are lower-value A shades. Value is often thought of as the most important colour aspect.

Studies have indicated that tooth colour, in adult teeth, is determined primarily by Dentine. The enamel layer plays a very minor role in the actual tooth colour.


- In young patients, teeth are brighter (higher value) and less translucent. With age, the enamel layer thins, exposing more Dentine, so teeth appear darker, particularly in the gingival third.
- Areas of highest intensity of colour (chroma) will be in the gingival region of the tooth due to a thinner enamel layer, so the Dentine is more visible.
- The Body region is a combination of the Dentine colour and the slight contribution by the enamel layer colour and surface morphology. Literature suggests that the intensity of the body is 1–2 shades lighter than the gingival area.
- The incisal area exhibits a high degree of translucency as the amount of Dentine present is decreased toward the incisal edge.

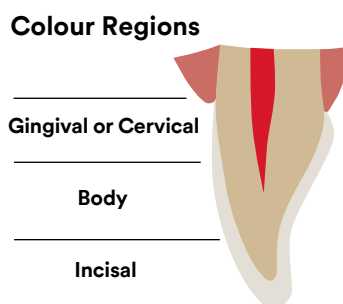

Opacity Considerations

When light contacts a tooth:

- Enamel diffuses and transmits light. If the Dentine layer is very thin or if there is no Dentine behind the enamel layer (as in the incisal edge), some of the light is transmitted through the tooth to the oral cavity. The oral cavity can reflect light back through the enamel.
- When light encounters Dentine, some of the light is absorbed and some is reflected back through the enamel.
- The light that is reflected and refracted back to the eye produces the colour of the tooth.
- The surface texture of a tooth plays a role in the perceived colour, i.e., a smoother surface will appear whiter (or higher value) than an irregular surface.

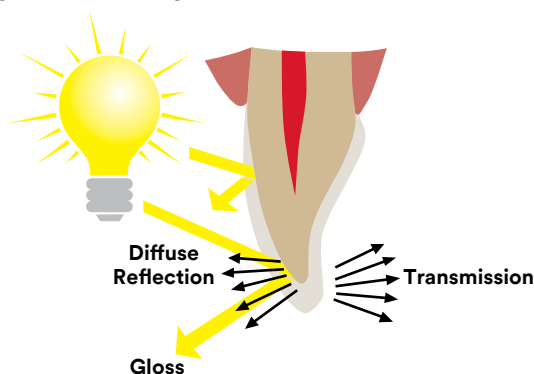

Opinion Leaders

Eighteen opinion leaders were invited to share their views regarding case presentations (recommended treatment and technique), education methods, strengths and weaknesses of current composites and shade guide offerings. Key findings are detailed below.

- It is important to gain agreement between patient and dentist as to the level of aesthetics required.
- Shade guides can be used to start the shade selection process; however, shade mock-ups, using the composite *in vivo*, are the best way to determine which composite shades are needed to blend with surrounding dentition.
- The acceptability of the resultant restorations can be influenced by many factors, including shades selected, depth of colour and re-creation of the natural tooth appearance (e.g., provided by layering translucent materials over less translucent materials or creating appropriate translucency along incisal edge), surface polish and surface morphology and patients' and dentists' preferences.

Shade Selection Tips and Hints for 3M™ Filtek™ Supreme XTE Universal Restorative

1. After pumicing the surface to remove any extrinsic stains, determine the shades needed for the restoration prior to tooth preparation or rubber dam placement. A tooth that is desiccated will be lighter than normal. Therefore, a shade taken on a desiccated tooth will be lighter than the tooth upon rehydration.
2. During shade selection,
 - If one shade is to be used,
 - Select the Body shade by examining the center (body) portion of the tooth. Choose the composite shade most closely approximating the center portion of the VITA classical shade tab.
 - If more than one shade is to be used to mimic actual tooth structure and increase the vitality of the final restoration, either use the shade wheel (next page) or identify which opacities are to be used. To determine which shade to choose in a given opacity:
 - Select the Dentine (or Body) shade by examining the exposed Dentine or the gingival area of the tooth. Choose the composite shade most closely approximating the cervical portion (grinding off the neck of the tab has been recommended by some) of the VITA classical shade tab.
 - Select the Body shade by examining the center (body) portion of the tooth. Choose the composite shade most closely approximating the center portion of the VITA classical shade tab.
 - Select the Enamel shade by examining the proximal or incisal area of anterior teeth, or from the cusp tips of posterior teeth. Choose the composite shade most closely approximating the center portion of the VITA classical shade tab.
 - A Translucent shade (in the same colour family) may be used to impart high translucency and increase the “depth” of the restoration.
3. Do a mock-up of the restoration prior to etching. The colour of a composite will be affected by its thickness. Composites may change colour upon curing. Place and cure composite material in the approximate thickness and area of the planned restoration. Obtain agreement with the patient of shade match. Remove mock-up easily by flicking it off the tooth with an explorer.
4. Evaluate shade match of the tabs and mock-up under different lighting conditions.
5. When finishing and polishing the restoration, mimic the surface morphology of adjacent teeth.

Shade Wheel

To aid in the shade selection process, 3M™ Filtek™ Supreme XTE Universal Restorative incorporates a unique (patented) shade selector wheel. Once a shade has been selected using the VITA classical Shade Guide, the selector offers recommendations for single-shade, two-shade or multi-shade restorations in supported and unsupported restorations (Figure 4).



Figure 4: Shade wheel: unsupported and supported restoration.



Figure 5: Shade recommendation.

Figure 5 indicates the proposed shade combinations for a Class IV and other unsupported restorations determined to be shade A2. Several options are offered, with final choice depending upon the size and aesthetic requirements of the restoration.

Simpler shade recommendations are given for restorations that are supported by tooth structure. Posterior restorations are an ideal place to start exploring the aesthetic options offered by the shade layering technique.

To use the wheel:

- Select VITA shade: Choose the composite shade most closely approximating the center portion of the VITA classical shade tab.
- Select the appropriate wheel side that corresponds to the type of restoration—e.g., supported or unsupported (Figure 4).
- Rotate the disc so that the VITA shade is visible in the innermost circle.
- Follow the 3M™ Filtek™ Supreme XTE Universal Restorative shade combination recommendations outlined for Single, Dual or Multi shades (Figure 5).

It should be noted that this tool is a guide only. Final results will be influenced by the thickness of composite layers, surrounding tooth structure, adjacent teeth, etc. Further, the layering diagrams depicted on the shade guide are offered as potential solutions in creating certain aesthetic effects. For instance, the Translucent shade may be applied internally as indicated to create translucency at the incisal third of a Class IV restoration. Alternatively, while not diagrammed, the Translucent shade may be applied as the last facial or occlusal increment to create depth. As using the Translucent shade in this manner may tend to decrease the overall value of the restoration, choosing a shade one step lighter for the increment immediately below the Translucent shade may moderate this effect.

Background

Fillers

Microfills

Traditional microfills are made from fumed silica, prepared by a pyrogenic process, with an average particle size of 0.04 μm . Typically, the primary particles tend to aggregate (the degree of aggregation varies, depending on the filler used in the microfill product). Breakdown of any aggregated particles into smaller entities is difficult, if not impossible, to achieve. The structure of these aggregates results in relatively low filler loading.

In the SEM (Figure 6), courtesy of Dr. Jorge Perdigao,⁹ the surrounding resin matrix was removed with a solvent.¹⁰ The field of view of this SEM did not include any of the prepolymerised filler, but focused instead on the individual silica aggregates. Note that the particles appear to be in the 0.1 μm range, significantly larger than 0.04 microns, as a result of the aggregation. Most microfill manufacturers add prepolymerised filled resin particles to increase filler loading. Prepolymerised filler is made by adding the fumed silica filler to resin. The mixture is polymerised and then ground to form particles. These ground particles are added to more resin and fumed silica filler. Even by using this process, microfills still have a substantially lower filler loading than hybrids, resulting in lower strength and wear resistance.

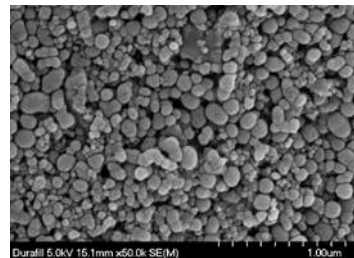


Figure 6: Durafill® VS.

Residual methacrylate groups bind the prepolymerised particles to the resin matrix. The effectiveness of this bond is impacted by the amount of residual double bonds on the surface of these particles. During the polymerisation of the prepolymerised filler, the reaction is driven to near completion. Hence, the bond of the prepolymerised filler particles to the resin is weaker than desired and breakdown frequently occurs at this interface. Additionally, traditional microfills containing only silica filler are not radiopaque. These properties have limited the usefulness of microfills, particularly in the posterior area.

The AFM¹¹ (Figure 7) is a 3D image of the surface of a microfill after 6000 cycles of toothbrush abrasion. Microfills have proven to retain their polish (surface reflectivity) over time. The prepolymerised filler particles are marginally more wear resistant than the surrounding matrix, resulting in small surface irregularities.

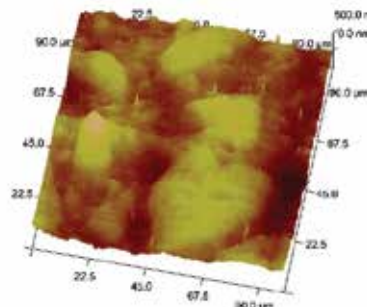


Figure 7: Durafill® VS.

Hybrids, Microhybrids and Nanohybrids

Hybrids, microhybrids and nanohybrids contain a broad distribution of particle sizes. A wide distribution of particle sizes can lead to high filler loading with resultant high strength and wear resistance. While they contain a small fraction of filler particles in the nanoparticle size range (less than 0.1 μ or 100 nm), they also contain a range of substantially larger filler particles, which influences the optical properties of these composites and detracts from polish retention (Figure 8). The average particle size of hybrids, microhybrids and nanohybrids is typically below 1 micron, but above 0.2 microns. The larger particle sizes can extend to well over 1 micron. They are typically manufactured by grinding or milling large fillers into smaller particles. The nanohybrids have some particles in the nanofiller size range less than 100 nm (0.1 μ m), but they also contain particles in the submicron range (0.2 to 1 μ m).

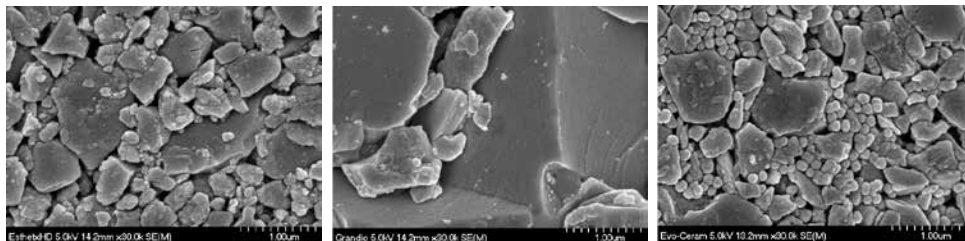


Figure 8: Left to right: EsthetX® HD High Definition Micro Matrix Restorative, Grandio®SO Universal Nano Hybrid Restorative and Tetric EvoCeram® Universal.

When any of these materials are subjected to abrasion, the resin between and around the particles is lost, leading to protruding filler particles (bumps). Eventually, the entire filler particle is plucked from the surface, resulting in craters. These bumps and craters create a roughened surface, resulting in loss of reflectivity (loss of polish retention) of the composite surface. The AFM images¹² (Figure 9) show the influence of the large- to small-particle ratios and the number of sizes of the particles after the surface has been toothbrush abraded. The material shown in the far right contains prepolymerised fillers, which are typically larger than the typical inorganic fillers. Note the roughness is clearly shown by the many peaks and valleys. The materials in the SEMs shown above correspond to the materials in the AFM images shown below.

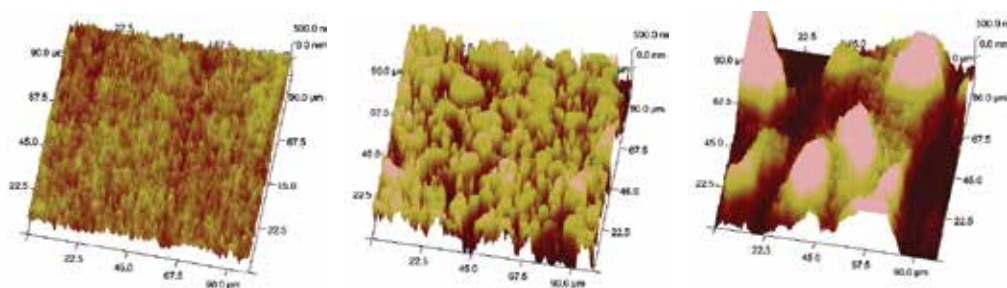


Figure 9: Left to right: EsthetX® HD High Definition Micro Matrix Restorative, Grandio®SO Universal Nano Hybrid Restorative and Tetric EvoCeram® Universal.

Nanocomposites

3M manufactures many of its fillers using a sol gel process. The sol gel process is a route wherein fillers are made from liquid precursors, or a “sol.” These liquids are chemically and mechanically processed to produce particles. One aspect of this process results in sintering, which effectively coalesces primary particles together to form larger filler particles. Sintering can be viewed as a type of melting process whereby the particles are softened, creating a surface which can attach to neighboring particles, resulting in a particle-to-particle bond. The sintering process can produce fillers that are highly densified or compacted, as found in 3M™ Filtek™ Z100™ Restorative and 3M™ Filtek™ Z250 Universal Restorative (Figure 10).

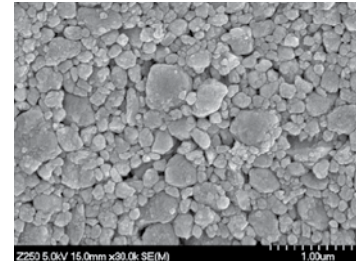


Figure 10: 3M™ Filtek™ Z250 Universal Restorative.

In 2002, 3M discovered a way to modify the sintering process to produce loosely agglomerated nanoparticles, i.e., nanoclusters. Although structurally different from densified particles, these nanoclusters behaved similarly to the densified particles found in other composites in terms of providing high filler loading. This resulted in a material with the strength and wear of hybrids with significantly improved polish retention and optical properties. This technology advance was used in 3M™ Filtek™ Supreme Universal Restorative.

Filtek Supreme restorative was formulated using both engineered nanoparticle and nanocluster fillers. The nanocluster filler particles consist of loosely bound aggregates of engineered nanofiller particles. The addition of engineered nanoparticles to formulations containing nanoclusters reduces the interstitial spacing of the filler particles, leading to higher filler loadings. The filled matrix (resin plus engineered nanoparticles) is harder and more wear resistant than resin alone. The increased filler loading results in better physical properties and wear resistance. The DEB shade fillers (Figure 11) of Filtek Supreme restorative were compositionally different than the T shade fillers (Figure 11). The nanoclusters in the DEB shades were zirconia/silica (thereby producing a radiopaque material), while the T shades contained silica clusters (hence, no radiopacity). The ratio of nanoclusters to engineered nanoparticles was different for the DEB shades than for the T shade in Filtek Supreme restorative. Nanoclusters comprised about 90% of the filler in the DEB shades, but only 50% of the filler in the T shades. The AFM images¹³ show the surfaces after they were toothbrush abraded. The Z scale is smaller in these images than in the AFM images shown previously, which effectively increases the magnification of the surface. During abrasion, the wear rate and wear pattern of the clusters is closer to the wear rate of the surrounding filled matrix, particularly in the 3M™ Filtek™ Supreme XT Universal Restorative Translucent shades (Figure 12). This increases the polish retention of the cured composite when compared to traditional hybrid composites.

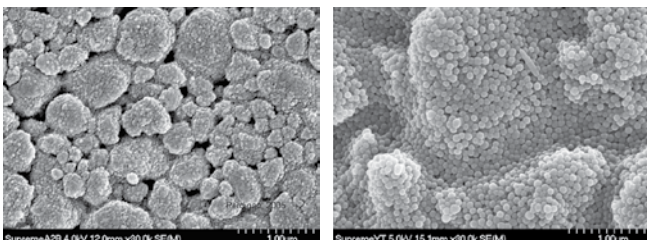


Figure 11: Left to right: 3M™ Filtek™ Supreme XT Universal Restorative (DEB shades) and Filtek Supreme XT restorative (T shades).

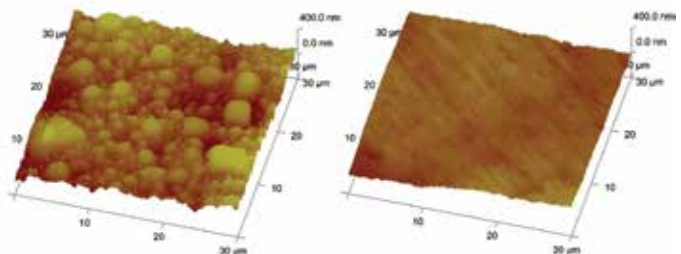


Figure 12: After abrasion, left to right: 3M™ Filtek™ Supreme XT Universal Restorative (DEB shades) and Filtek Supreme XT restorative (T shades).

Filler Improvements in 3M™ Filtek™ Supreme XTE Universal Restorative

This filler technology was improved again. The manufacturing process, where the clusters are formed, was modified to produce less sintering. Once again, the nanoclusters are produced in a broad range of sizes, enabling a high filler loading. As the particles are not as strongly sintered, the cluster size range could be broadened (vs. 3M™ Filtek™ Supreme XT Universal Restorative) without affecting properties such as polish retention. These nanoclusters still have the structural integrity to provide strength, fracture and wear resistance. In the SEMs (Figure 13),⁹ note the shape of the primary nanoparticles are still evident in the clusters. Both materials (DEB and T shades) contain zirconia/silica clusters (Figure 14), silica nanoparticles and zirconia nanoparticles. The ratio of nanoclusters to nanoparticles is similar in both formulations. Compositionally, both clusters are the same. In order to achieve the high degree of transparency and opalescence required for the T shades, the manufacturing process is slightly different. Both the DEB shades and the T shades are radiopaque. During abrasion, their wear rate and pattern are more similar to the nanofilled matrix surrounding the clusters than Filtek Supreme Plus restorative DEB and T shades. Note that in the AFM 3D image (Figure 15), the Z-scale is different than previous AFM images, resulting in a greater magnification of these surfaces. This greater magnification exacerbates the very slight irregularities in the surfaces.

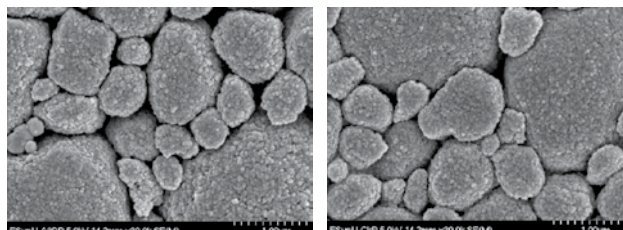


Figure 13: Left to right: nanoclusters at 30,000x 3M™ Filtek™ Supreme XTE Universal Restorative (DEB shades) and Filtek Supreme XTE restorative (T shades).

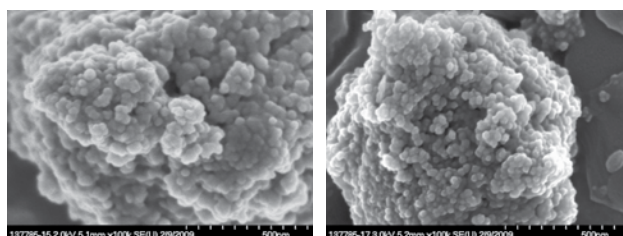


Figure 14: Left to right: nanoclusters at 100,000x 3M™ Filtek™ Supreme XTE Universal Restorative (DEB shades) and Filtek Supreme XTE restorative (T shades).

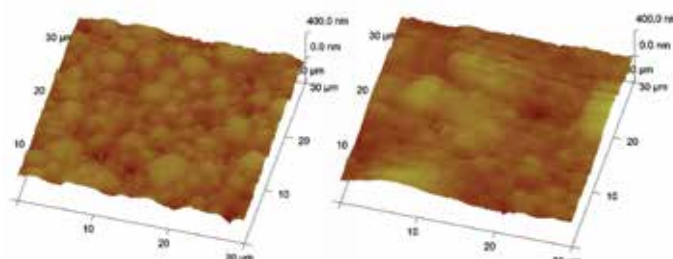


Figure 15: Left to right: after abrasion, 3M™ Filtek™ Supreme XTE Universal Restorative (DEB shades) and Filtek Supreme XTE restorative (T shades).

Resin System

The resin system introduced with 3M™ Filtek™ Z250 Universal Restorative and used in 3M™ Filtek™ Supreme XT Universal Restorative comprises the majority of the 3M™ Filtek™ Supreme XTE Universal Restorative resin system. The resin consists of three major components. The majority of TEGDMA (in the 3M™ Z100™ Restorative system) was replaced with a blend of UDMA (urethane dimethacrylate) and Bis-EMA(6) (Bisphenol A polyethylene glycol diether dimethacrylate). UDMA and Bis-EMA(6) resins are of higher molecular weight than TEGDMA and therefore have fewer double bonds per unit of weight. The high molecular weight materials also impact the measurable viscosity. However, the higher molecular weight of the resin results in less shrinkage, improved aging and a slightly softer resin. TEGDMA and PEGDMA are used in minor amounts to adjust the viscosity. PEGDMA was used to replace part of the TEGDMA component to moderate shrinkage in Filtek Supreme XTE restorative.

In Vitro Handling Evaluations

During the years 3M™ Filtek™ Supreme Universal Restorative has been on the market, dentists have commented favorably on the handling of the Dentine, Enamel and Body shades. As such, when dentists and opinion leaders were asked to identify features to improve in this iteration, they indicated the handling acceptability needed to be maintained. At the same time, they indicated the handling of the Translucent shades needed to be improved.

Handling of composites is influenced by both resin and filler. While the filler composition of Filtek Supreme XTE restorative Dentine, Enamel and Body shades is similar to its predecessor, the morphology of the clusters is different. Both the filler composition and morphology were modified to produce the new Translucent shade formulation.

Hence, numerous handling evaluations were conducted throughout the development process with dentists. Blind evaluations were done with anterior and posterior restoration in heated typodonts. Dentists were asked a series of questions about the handling of each paste. There were over 500 evaluations of this type conducted. Filtek Supreme XT restorative was included as a blind control in these evaluations. Overall, the handling of Filtek Supreme XTE restorative met or exceeded the acceptability of the handling of Filtek Supreme XT restorative DEB shades. The handling acceptability of the T shades of Filtek Supreme XTE restorative exceeded that of Filtek Supreme XT restorative T shades.

In one *in vitro* study, dentists were asked to evaluate a series of pastes that included different lots of 3M™ Filtek™ Supreme XTE Universal Restorative representing potential handling targets and two lots of 3M™ Filtek™ Supreme XT Universal Restorative (Figure 16). About one-third of the evaluators were current Filtek Supreme XT restorative users. The materials were evaluated in random order, restoring a Class II and Class IV preparation on heated typodonts. The handling acceptance of the DEB shade pastes is shown in Figure 16. Greater than 70% of the dentists evaluating these materials liked the handling, and consequently identified the handling specification range. In addition to the overall acceptability, the following handling attributes were also rated: viscosity, stickiness to instrument, flow, ability to hold shape or resist slump, ease of veneering (for anterior restorations), cavity and marginal adaptation, and packability (for posterior restorations only). In all cases, the Filtek Supreme XTE restorative materials were rated as the same or better than the Filtek Supreme XT restorative materials.

An evaluation comparing the two Translucent shade formulations yielded even better results. A similar method was followed but with three Filtek Supreme XTE restorative Translucent shade lots representing different potential handling targets and one Filtek Supreme XT restorative Translucent shade lot. Nominally, twice as many dentists liked the handling of Filtek Supreme XTE restorative T shade lots as Filtek Supreme XT restorative T shades. (Figure 16) In addition, significant improvements were also noted in the individual handling attributes: viscosity, stickiness to instrument, flow, ability to hold shape or resist slump, and ease of veneering.

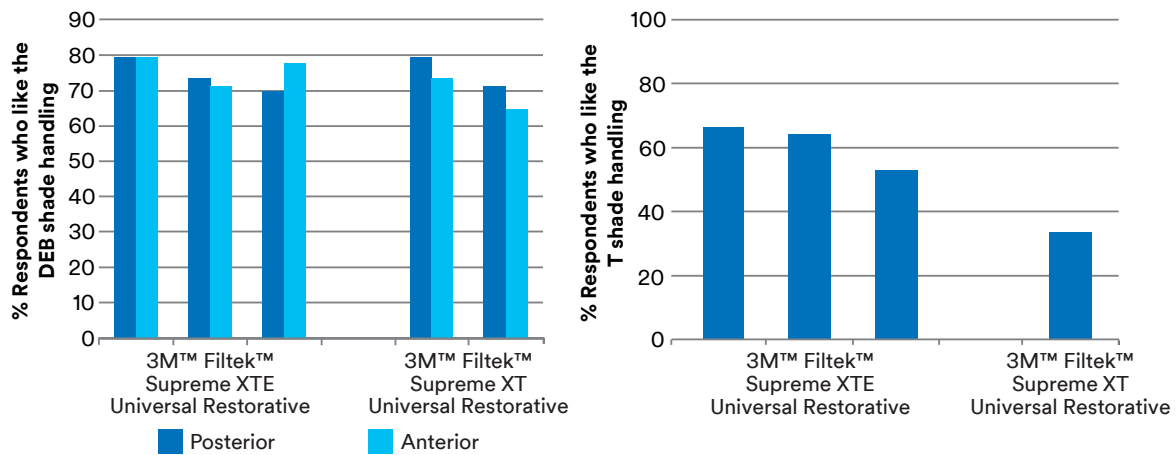


Figure 16: Handling Acceptability. Source: 3M internal data

Physical Properties

Polish Retention

Toothbrush Abrasion

Composite materials were shaped into tiles and thoroughly cured. The surfaces were polished wet using a Beuhler variable-speed grinder-polisher to remove the air-inhibited layer and to ensure a uniform surface. They were stored in water at 37°C for 24 hours. Gloss was measured. The samples were brushed with toothpaste and a toothbrush that was mounted on an Automatic Toothbrush Machine. Gloss measurements were taken after 500 cycles and then every 1,000 cycles. The test was terminated after 6,000 toothbrush strokes.

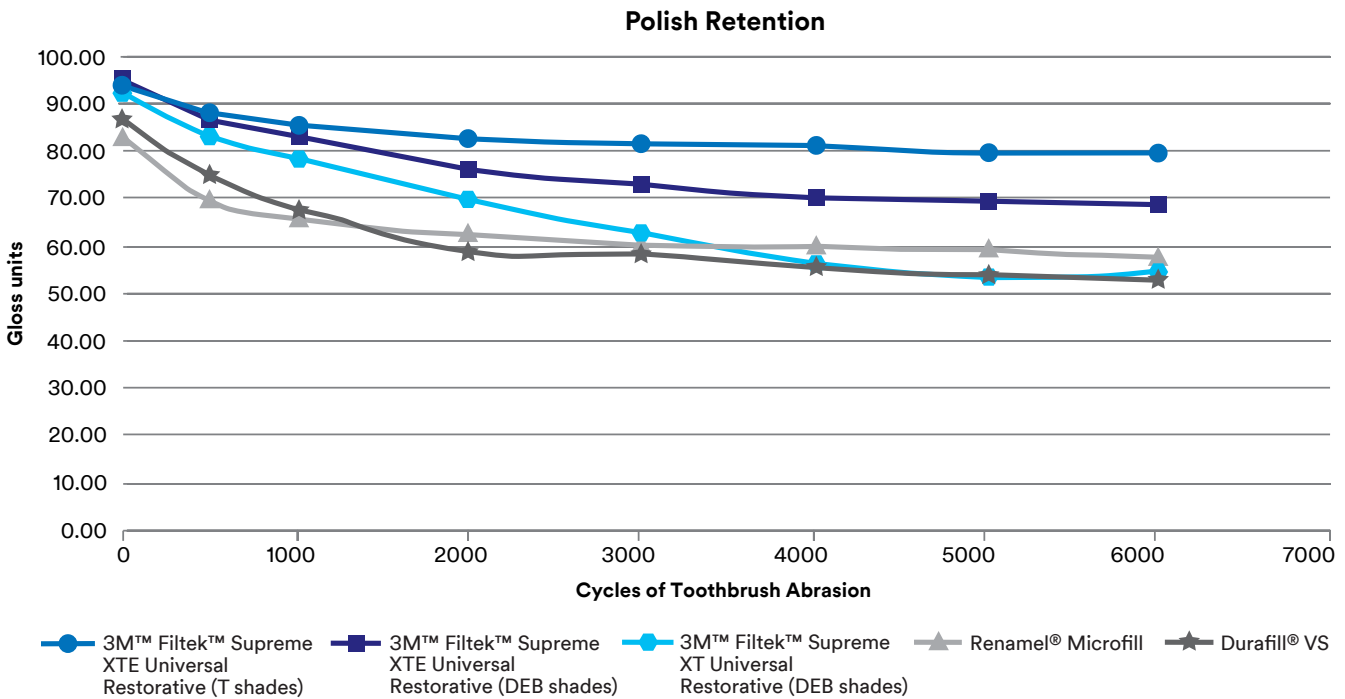


Figure 17: Polish retention versus microfills. Source: 3M internal data

- In this test, even after only 500 cycles of toothbrush abrasion, the polish retention (gloss) of 3M™ Filtek™ Supreme XTE Universal Restorative DEB shades and T shades was statistically significantly higher than the microfill products Durafill® VS and Renamel® Microfill and the hybrid composites Ceram-X™ Nano Ceramic Restorative, Estelite® Sigma Quick, EsthetX® HD High Definition Micro Matrix Restorative, Gradia® Direct X, Grandio®SO Universal Nano Hybrid Restorative, Herculite® XRV Ultra™, Premise™ Universal Composite, Tetric EvoCeram® Universal, TPH® 3flow Liquid Micro Hybrid Restorative and Venus®.
- Both compositions of Filtek Supreme XTE restorative were better in gloss than 3M™ Filtek™ Supreme XT Universal Restorative after 2,000 cycles of toothbrush abrasion.
- After 6,000 cycles, the gloss of Filtek Supreme XTE restorative T shades was better than Durafill® VS, Renamel® Microfill, Ceram-X™ Nano Ceramic Restorative, Estelite® Sigma Quick, EsthetX® HD High Definition Micro Matrix Restorative, Gradia® Direct X, Grandio®SO Universal Nano Hybrid Restorative, Herculite® XRV Ultra™, Premise™ Universal Composite, Tetric EvoCeram® Universal, TPH® 3flow Liquid Micro Hybrid Restorative and Venus®.
- After 6,000 cycles, the gloss of Filtek Supreme XTE restorative DEB shades was statistically better than Durafill® VS, Renamel® Microfill, Ceram-X™ Nano Ceramic Restorative, EsthetX® HD High Definition Micro Matrix Restorative, Gradia® Direct X, Grandio®SO Universal Nano Hybrid Restorative, Herculite® XRV Ultra™, Premise™ Universal Composite, Tetric EvoCeram® Universal, TPH® 3flow Liquid Micro Hybrid Restorative and Venus®.


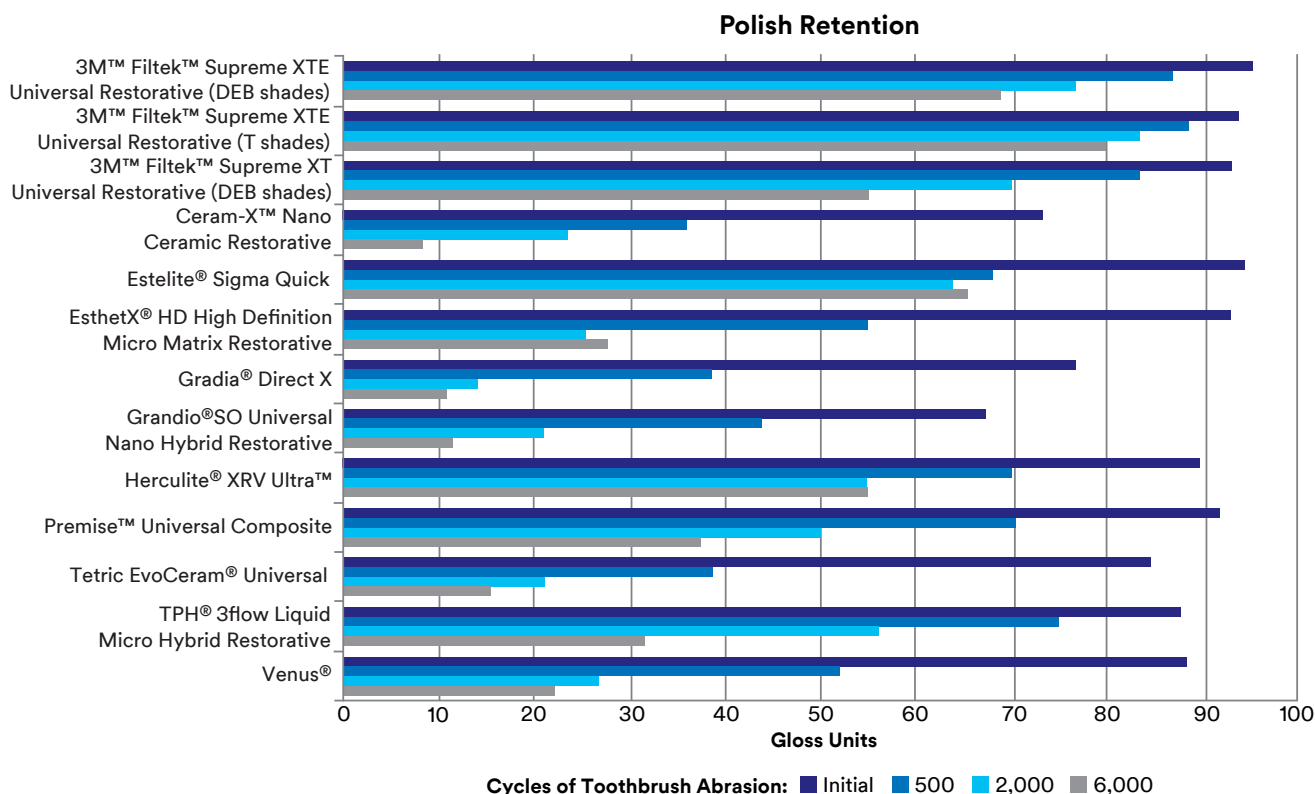


Figure 18: Polish retention versus other universal restoratives. Source: 3M internal data


Wyko Images

These images were generated using a Wyko Optical profiler. This method provides a wider field of view than the previous AFM images. The bar to the right of the scanned image identifies the colour coding key of the images.

The surface roughness is shown by the colour differences. Blue indicates pits, and red indicates protrusions from the plane of the sample. Shades of green indicate roughness with a smaller peak-to-valley range.

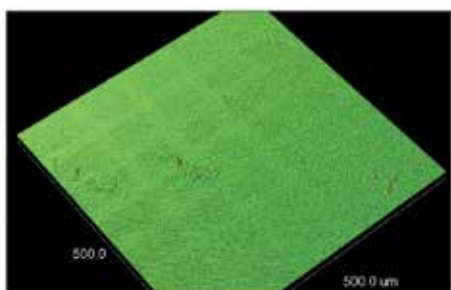


DEB shades

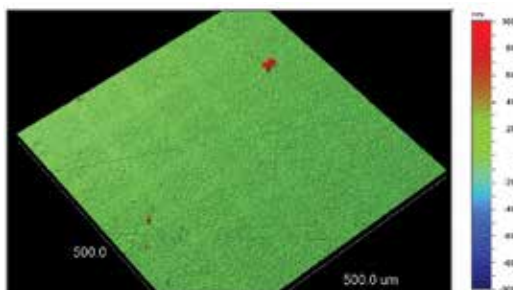


T shades

Polished: 3M™ Filtek™ Supreme XTE Universal Restorative.

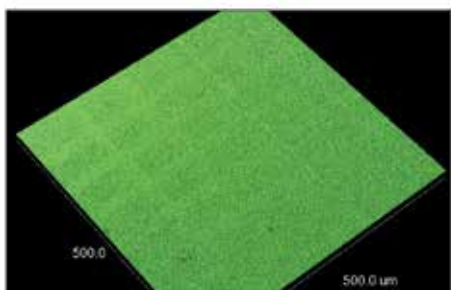


DEB shades

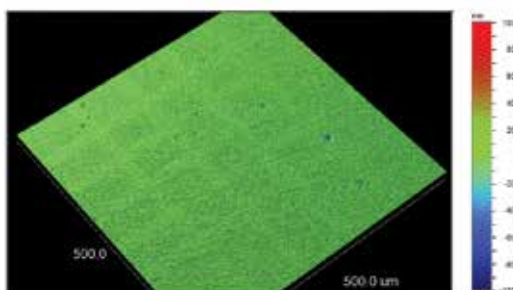

T shades

Polished: 3M™ Filtek™ Supreme XT Universal Restorative.

Note the smoothness of the surfaces after polish. In all of the images above, there is little colour variation, indicating little roughness ($Ra^{14} < 20$ nm).

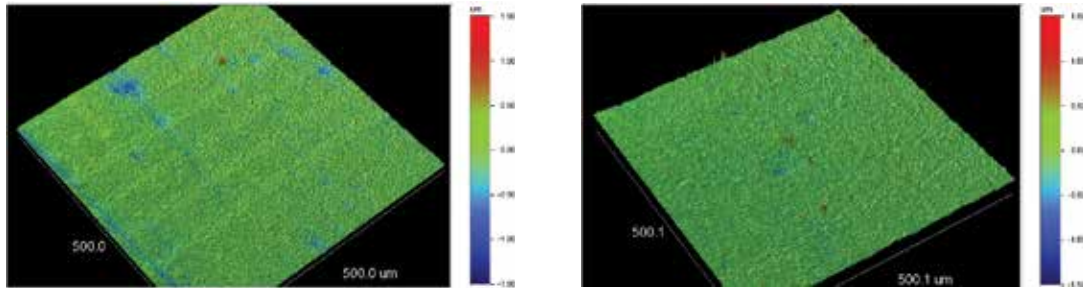


DEB shades

T shades

Toothbrush abraded: 3M™ Filtek™ Supreme XTE Universal Restorative.

After 6,000 cycles of toothbrush abrasion, Wyko images were taken and the scale was changed to a slightly smaller magnification. The surfaces of the 3M™ Filtek™ Supreme XTE Universal Restorative DEB (Ra~129 nm) and T shade (Ra~70 nm) samples exhibit very minor colour variation across the samples.

The images below show the original 3M™ Filtek™ Supreme XT Universal Restorative DEB and T shades (Ra~148 nm) after toothbrush abrasion. Note the few deeper blue areas where larger masses, probably clusters, were removed during toothbrush abrasion.

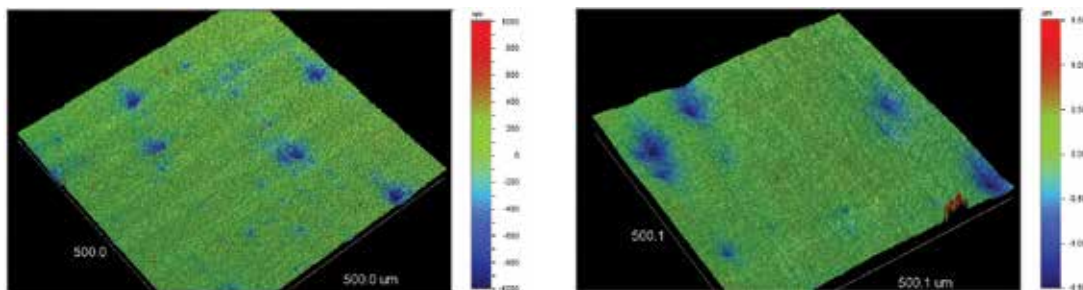


DEB shades

T shades


Toothbrush abraded: 3M™ Filtek™ Supreme XT Universal Restorative.

Below are images generated of two microfill restoratives after toothbrush abrasion. Note in both samples the higher areas due to the prepolymerised filler particles abrading at a different rate than the surrounding resin matrix (Ra~135 nm). Note the deeper blue areas where larger masses were removed, which is similar to 3M™ Filtek™ Supreme XT Universal Restorative materials.

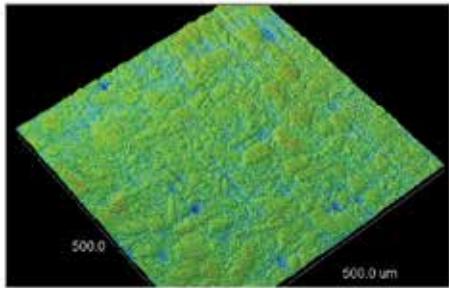


Durafill® VS

Toothbrush abraded: microfills.

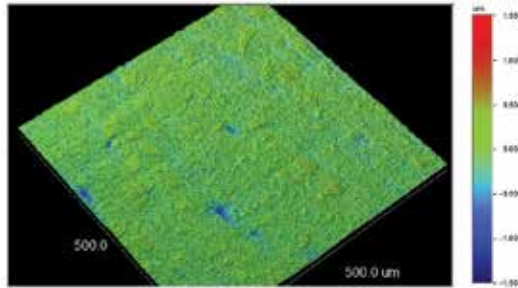


Renamel® Microfill


In the Ceram-X™ Nano Ceramic Restorative image below, there is a significant roughness indicated due to the ragged appearing edges of the image and the yellow-orange hue of the surface (Ra~240 nm). The EsthetX® HD High Definition Micro Matrix Restorative image exhibits a less uniform orange surface hue (Ra~187 nm). This indicates broader and larger concentrations of raised areas. Both have measurably greater surface roughness than 3M™ Filtek™ Supreme XTE Universal Restorative materials.

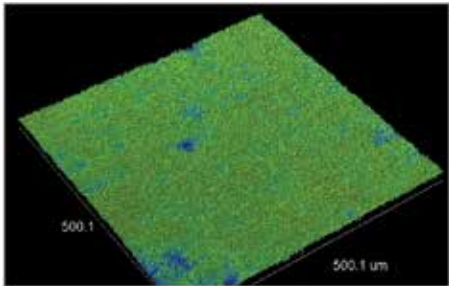

Ceram-X™ Nano Ceramic Restorative

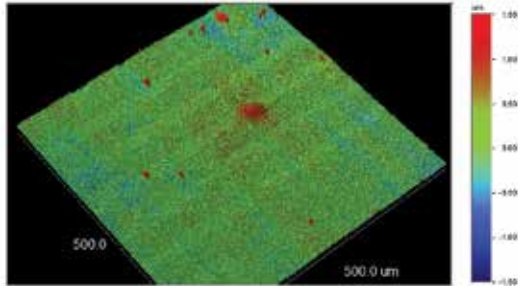


EsthetX® HD High Definition Micro Matrix Restorative

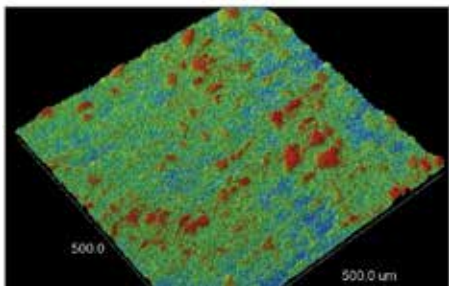


Gradia® Direct X

Toothbrush abraded: universals.

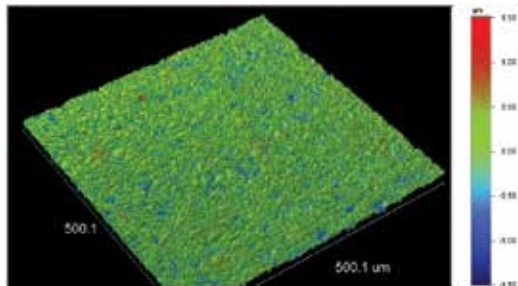


Grandio®SO Universal Nano Hybrid Restorative

Gradia® Direct X exhibits a very rough surface after toothbrush abrasions (Ra~287 nm). The Wyko image shows orange protrusions and deep blue valleys in the surface. The Grandio®SO Universal Nano Hybrid Restorative surface shows a smaller peak-to-valley ratio (Ra~226 nm) than Gradia® Direct X, but is still very rough (the colour across the sample is not uniform).

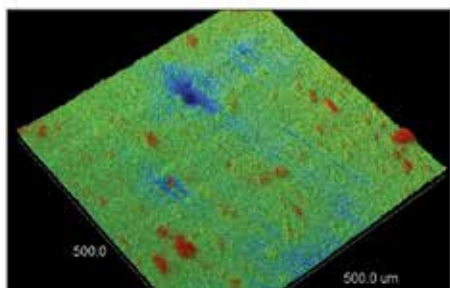

Herculite® XRV Ultra™

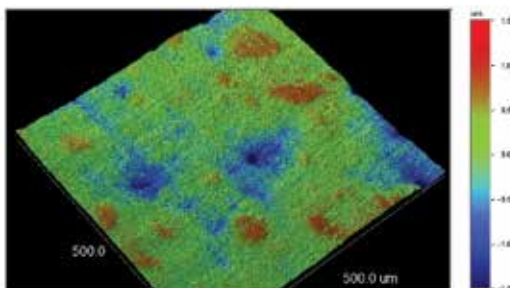


Premise™ Universal Composite


Toothbrush abraded: universals.

In both of the materials shown above, there are a significant number of bumps on the surface (peaks), which may be from filler particles protruding as the surrounding resin matrix was worn away (Herculite® XRV Ultra™ Ra~280 nm, Premise™ Universal Composite Ra~266 nm). In addition, Premise™ Universal Composite has several large valleys where a mass material was lost.

The prepolymerised filler particles (orange protrusions) in Tetric EvoCeram® Universal become readily apparent in this surface analytic technique (Ra~542 nm). The colour variation across the Tetric EvoCeram® Universal sample covers the entire range of this surface roughness analytic technique (+ 1.5um). TPH® 3flow Liquid Micro Hybrid Restorative, on the other hand, exhibits deep valleys (large particle loss) but more diffused peak areas (orange hues) (Ra~348 nm).

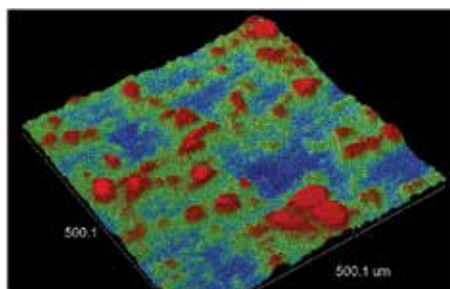


Tetric EvoCeram® Universal

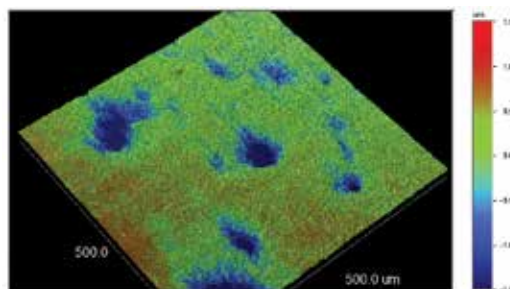

TPH® 3flow Liquid Micro Hybrid Restorative

The abrasion pattern of the Venus® sample is similar to that of Ceram-X™ Nano Ceramic Restorative. There is an obvious orange cast to the sample, indicating many peaks rising from the surface (Ra~147 nm). In addition, there are several deep blue striations that were created from the toothbrush abrasion test.


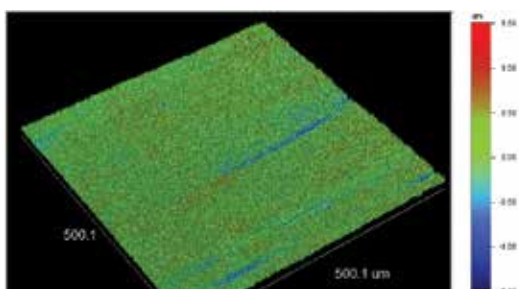


Venus®

Toothbrush abraded: universals.

3-Body Wear

The wear rate was determined by an *in vitro* 3-body wear test. In this test, composite (1st body) is loaded onto a wheel, which contacts another wheel, which acts as an “antagonistic cusp” (2nd body). The two wheels counter-rotate against one another, dragging abrasive slurry (3rd body) between them. Dimensional loss during 156,000 cycles is determined by profilometry at regular intervals (i.e., after every 39,000 cycles). As the wear in this method typically follows a linear pattern, the data is plotted using linear regression. The wear rates, i.e., the slope of the lines, are determined. The comparison of rates reduces some of the variability in the test due to sample preparation and can be predictive of anticipated wear beyond the length of the actual test.

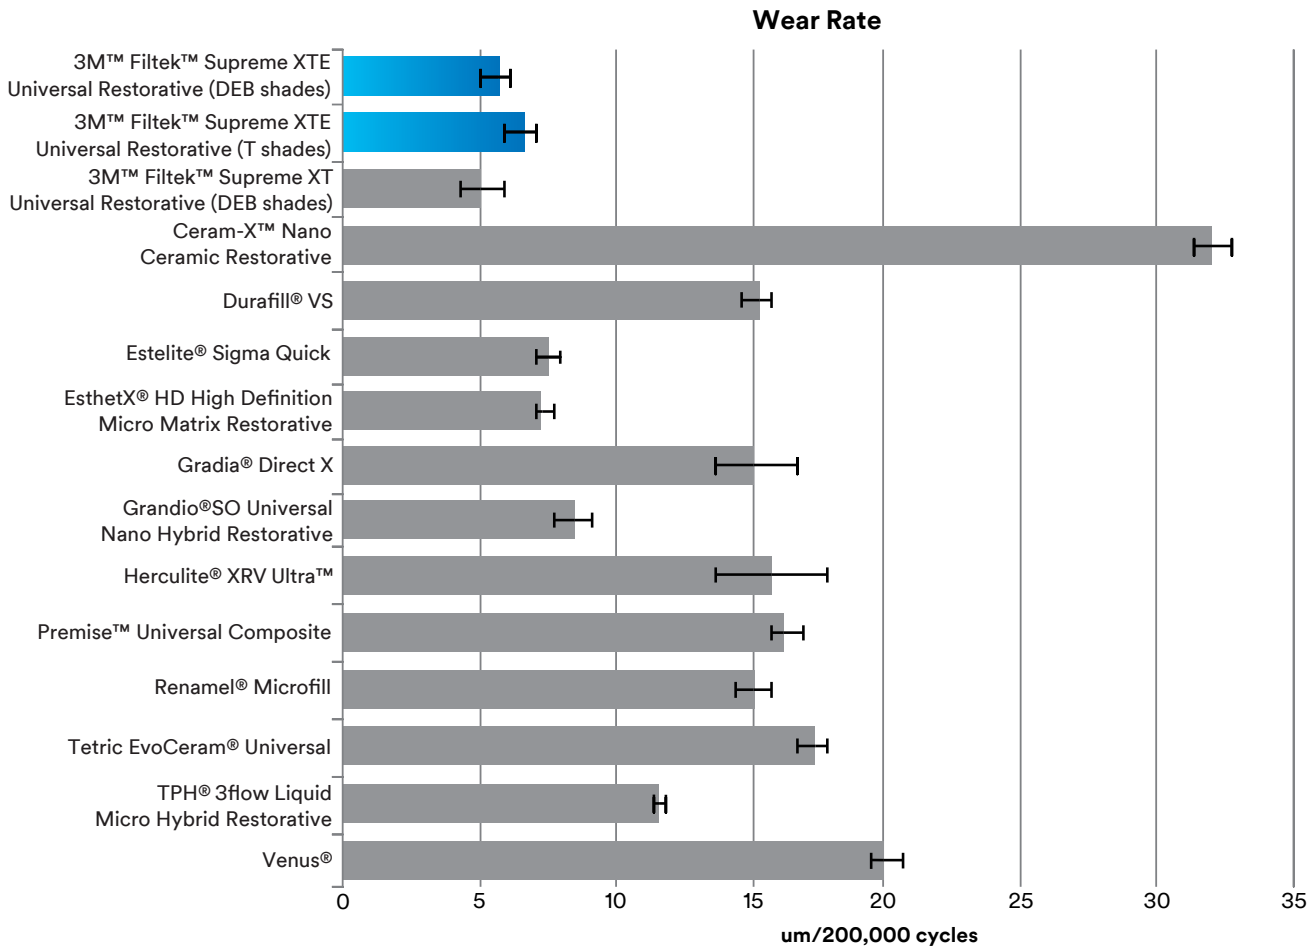



Wear rate. Source: 3M internal data

The lower the wear rate, the better the wear resistance. The wear rate of 3M™ Filtek™ Supreme XTE Universal Restorative DEB shades and T shades is comparable to the 3-body wear rate of 3M™ Filtek™ Supreme XT Universal Restorative. The 3-body wear rate is statistically significantly lower (more wear resistant) than the microfills Durafill® VS and Rename!® Microfill. In addition, it is statistically lower than Ceram-X™ Nano Ceramic Restorative, Estelite® Sigma Quick, EsthetX® HD High Definition Micro Matrix Restorative, Gradia® Direct X, Grandio®SO Universal Nano Hybrid Restorative, Herculite® XRV Ultra™, Premise™ Universal Composite, Tetric EvoCeram® Universal, TPH® 3flow Liquid Micro Hybrid Restorative and Venus® universal restoratives.

Fracture Toughness

The values reported for fracture toughness (K1c) are related to the energy required to propagate a crack. In this test, a short rod of material is cured. A notch is cut into the cylinder. The cylinder is placed on a fixture that supports either end and the stylus is positioned above the notch. This is similar to 3-point bend (similar to the fixture that provides flexural strength and modulus data).

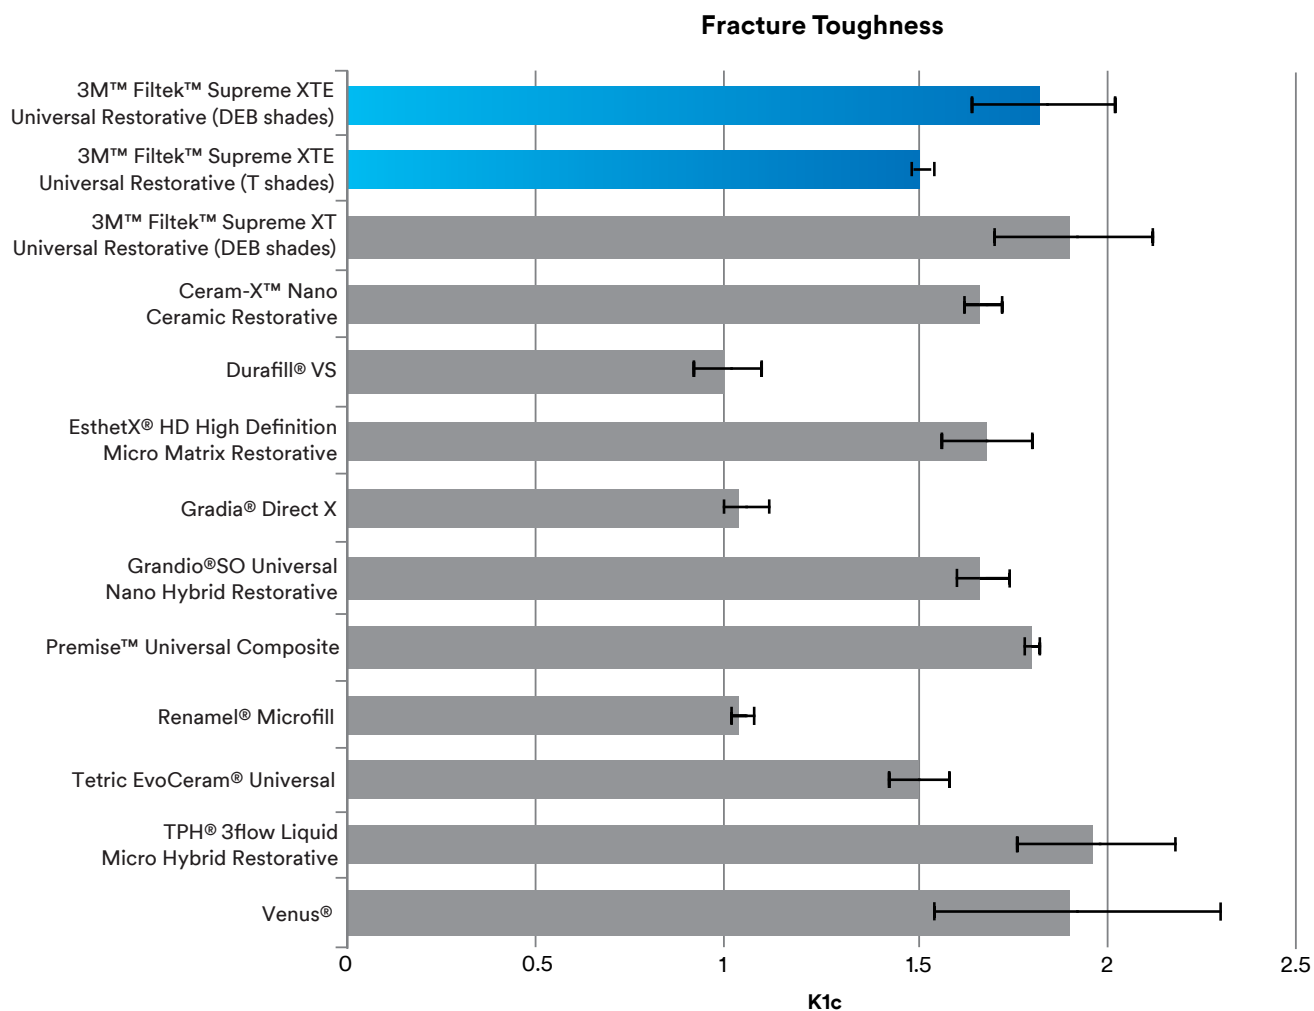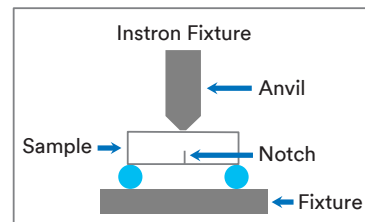


Fracture toughness. Source: 3M internal data

The fracture toughness of 3M™ Filtek™ Supreme XTE Universal Restorative (DEB shades) is comparable to 3M™ Filtek™ Supreme XT Universal Restorative. Filtek Supreme XTE restorative has statistically significantly higher fracture toughness than the microfills Durafill® VS and Renamel® Microfill. The fracture toughness of Filtek Supreme XTE restorative is also statistically significantly higher than Gradia® Direct X and Tetric EvoCeram® Universal.


Compressive and Diametral Tensile Strength

Compressive strength is particularly important because of chewing forces. Rods are made of the material and simultaneous forces are applied to the opposite ends of the sample length. The sample failure is a result of shear and tensile forces.




The compressive strength of 3M™ Filtek™ Supreme XTE Universal Restorative (DEB shades) is comparable to the T shades and 3M™ Filtek™ Supreme XT Universal Restorative. Filtek Supreme XTE restorative has statistically significantly higher compressive strength than Gradia® Direct X.

Compressive Strength

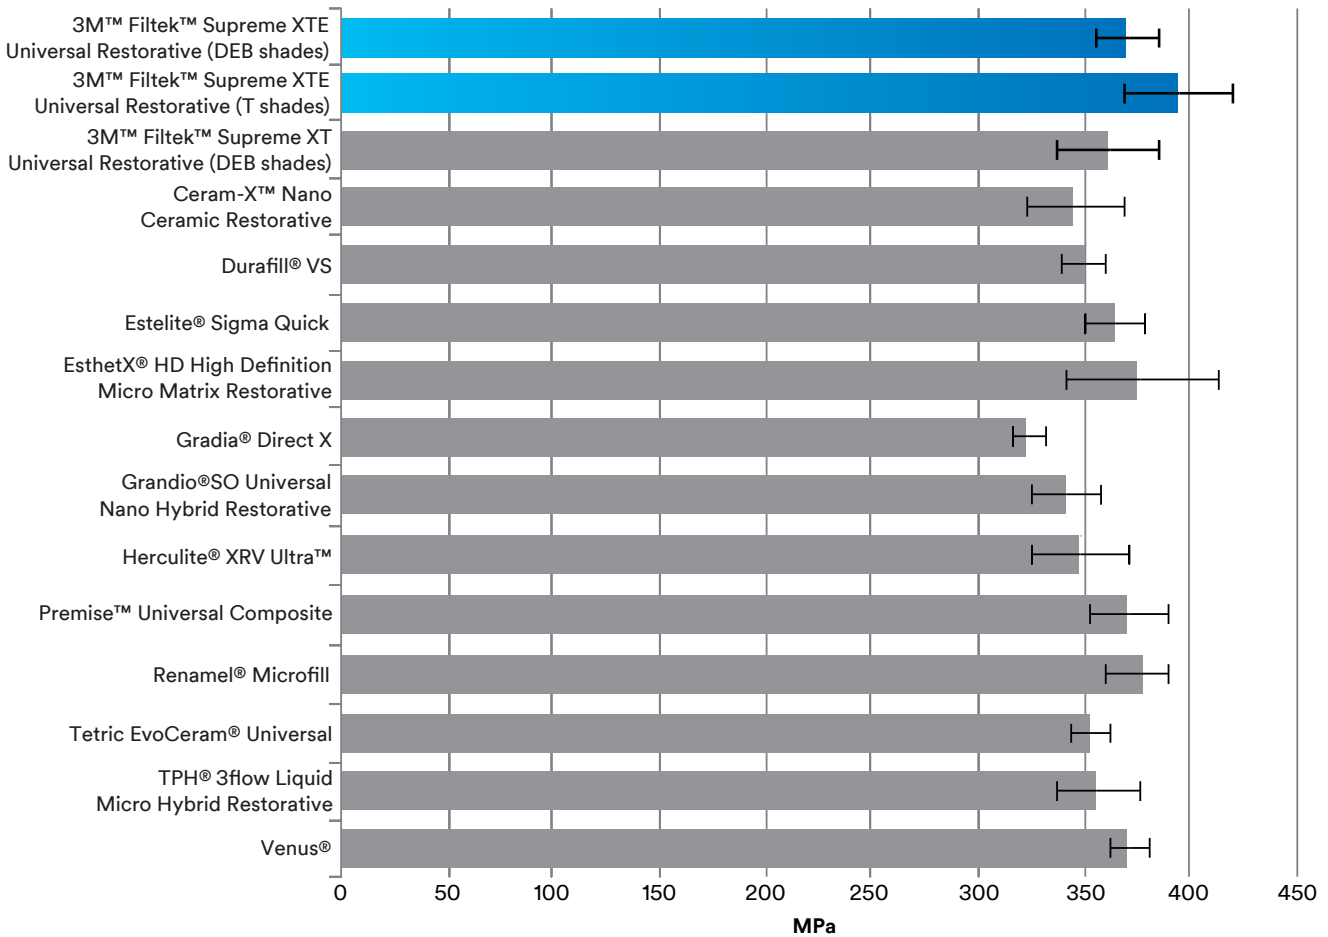


Compressive strength. Source: 3M internal data

Diametral tensile strength is measured using a similar apparatus. Compressive forces are applied to the sides of the sample, not the ends, until fracture occurs.




The diametral tensile strength of 3M™ Filtek™ Supreme XTE Universal Restorative is comparable to 3M™ Filtek™ Supreme XT Universal Restorative. The diametral tensile strength is statistically significantly higher than the microfills Durafill® VS and Renamel® Microfill. In addition, it is statistically higher than Ceram-X™ Nano Ceramic Restorative, Estelite® Sigma Quick, EsthetX® HD High Definition Micro Matrix Restorative, Gradia® Direct X, Premise™ Universal Composite, Tetric EvoCeram® Universal, TPH® 3flow Liquid Micro Hybrid Restorative and Venus® universal restoratives.

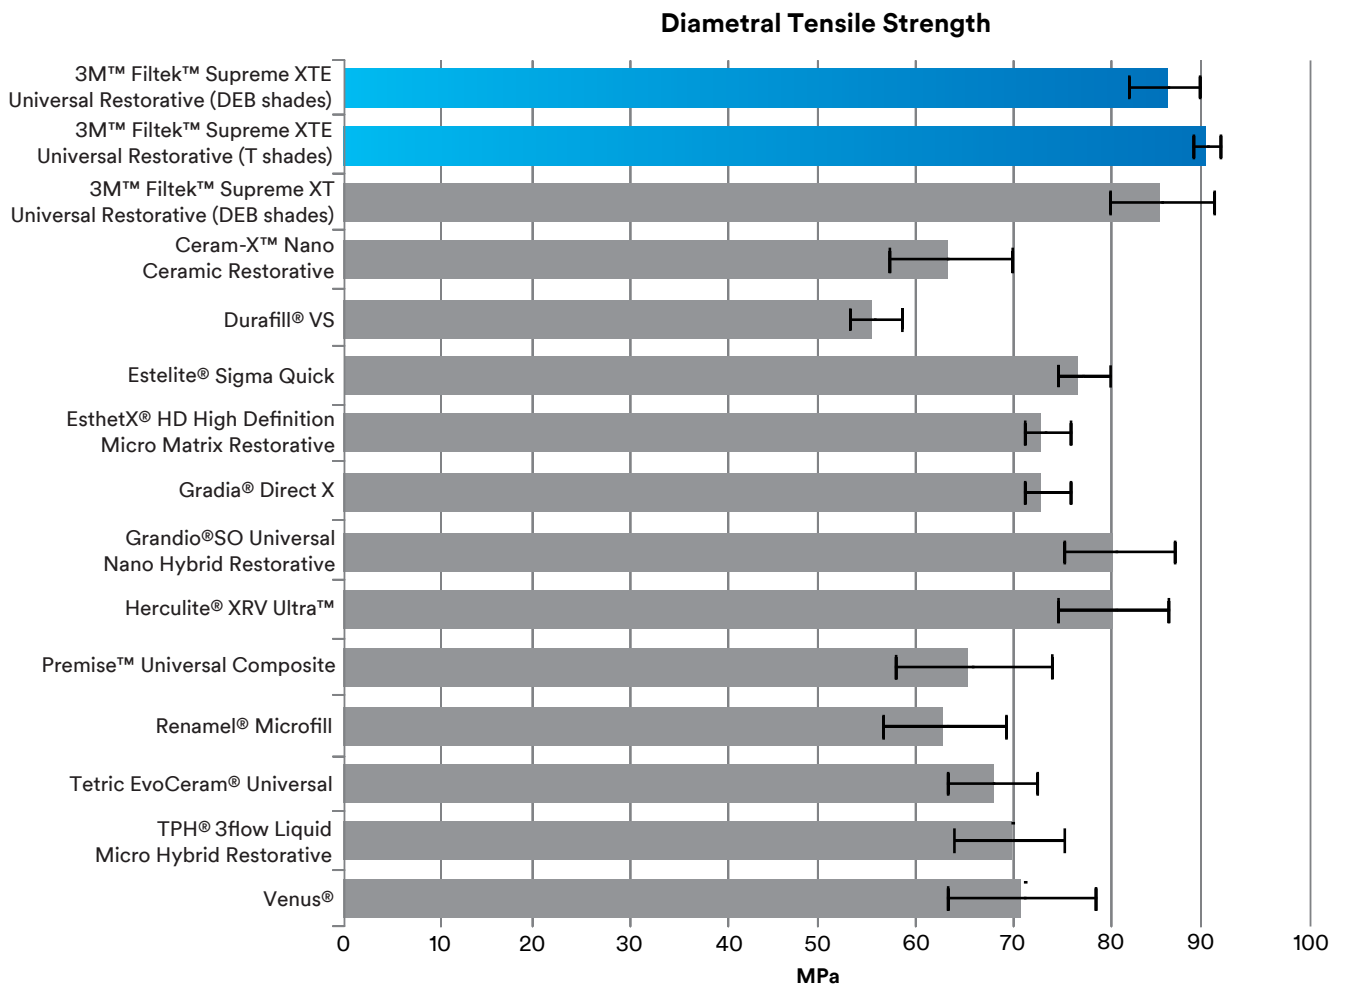


Diametral tensile strength. Source: 3M internal data

Flexural Strength and Modulus

Flexural strength is determined in the same test as flexural modulus. Flexural strength is the value obtained when the sample breaks. This test combines the forces found in compression and tension.




The flexural strength of the DEB shades of 3M™ Filtek™ Supreme XTE Universal Restorative is comparable to the T shades and 3M™ Filtek™ Supreme XT Universal Restorative. The flexural strength of Filtek Supreme XTE restorative is significantly higher than the microfills Durafill® VS and Renamel® Microfill. It is also higher than the universal restoratives Ceram-X™ Nano Ceramic Restorative, Estelite® Sigma Quick, EsthetX® HD High Definition Micro Matrix Restorative, Gradia® Direct X, Grandio®SO Universal Nano Hybrid Restorative, Herculite® XRV Ultra™, Premise™ Universal Composite, Tetric EvoCeram® Universal and Venus®.

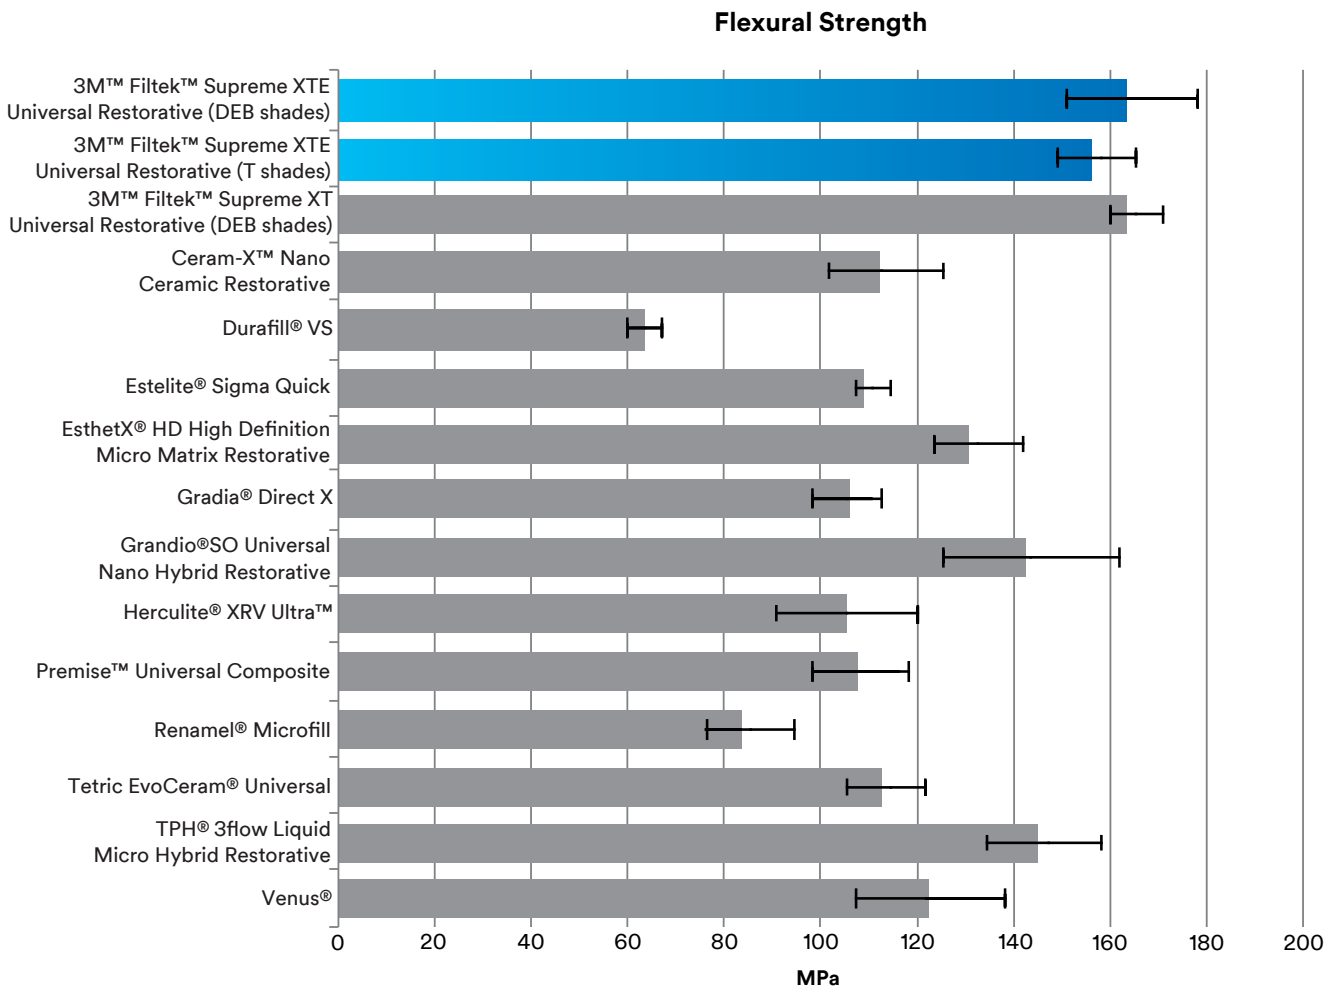


Flexural strength. Source: 3M internal data

Flexural modulus is a method of defining a material’s stiffness. A low modulus indicates a flexible material. The flexural modulus is measured by applying a load to a material specimen that is supported at each end.




The flexural modulus of the DEB shades of 3M™ Filtek™ Supreme XTE Universal Restorative is statistically different than the T shades, Ceram-X™ Nano Ceramic Restorative, Durafill® VS, Estelite® Sigma Quick, EsthetX® HD High Definition Micro Matrix Restorative, Gradia® Direct X, Grandio®SO Universal Nano Hybrid Restorative, Herculite® XRV Ultra™, Premise™ Universal Composite, Renamel® Microfill, Tetric EvoCeram® Universal, TPH® 3flow Liquid Micro Hybrid Restorative and Venus® restoratives. It is the same as 3M™ Filtek™ Supreme XT Universal Restorative.

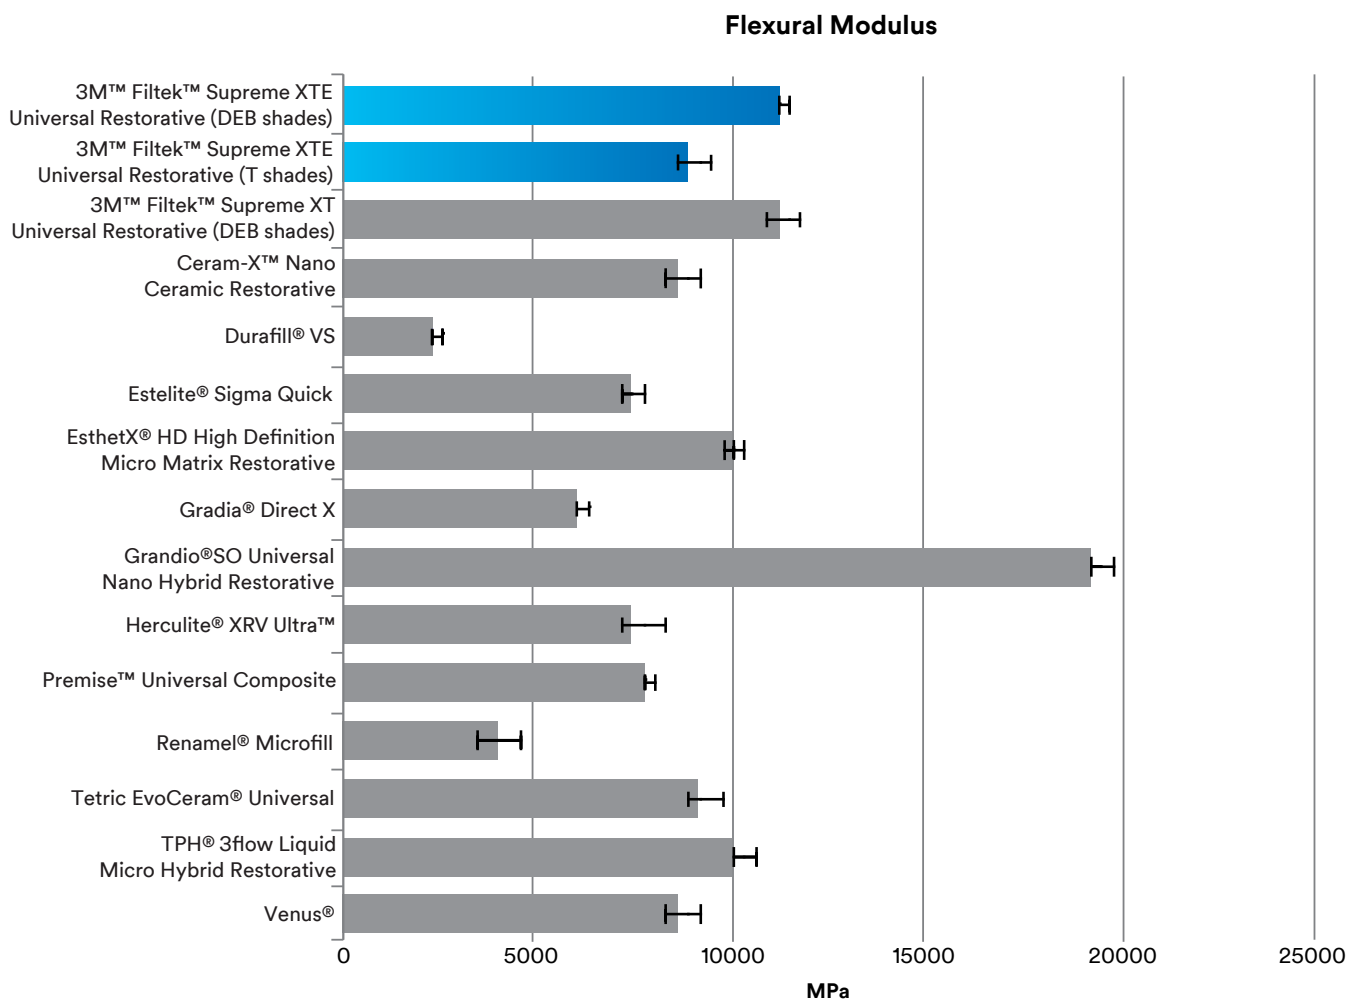


Flexural modulus. Source: 3M internal data

Volumetric Shrinkage

A method for determining polymerisation shrinkage was described by Watts and Cash.¹⁵ In this method, a disc-shaped test specimen and uncured paste is sandwiched between two glass plates and light cured through the rigid lower plate. The flexible upper plate is deflected during the polymerisation of the test specimen. The less the flexible plate bends, the lower the shrinkage. Deflection is measured and recorded as a function of time. Although this process actually measures linear shrinkage, volumetric shrinkage was closely approximated due to the fact that the dimensional changes were limited to the thickness dimension. The lower the value, the less the shrinkage.

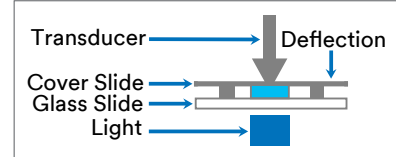

In this test, samples were exposed for 60 seconds to a 3M™ Visilux™ 2 Visible Light Curing Unit. The final shrinkage was recorded 4 minutes after the end of light exposure.

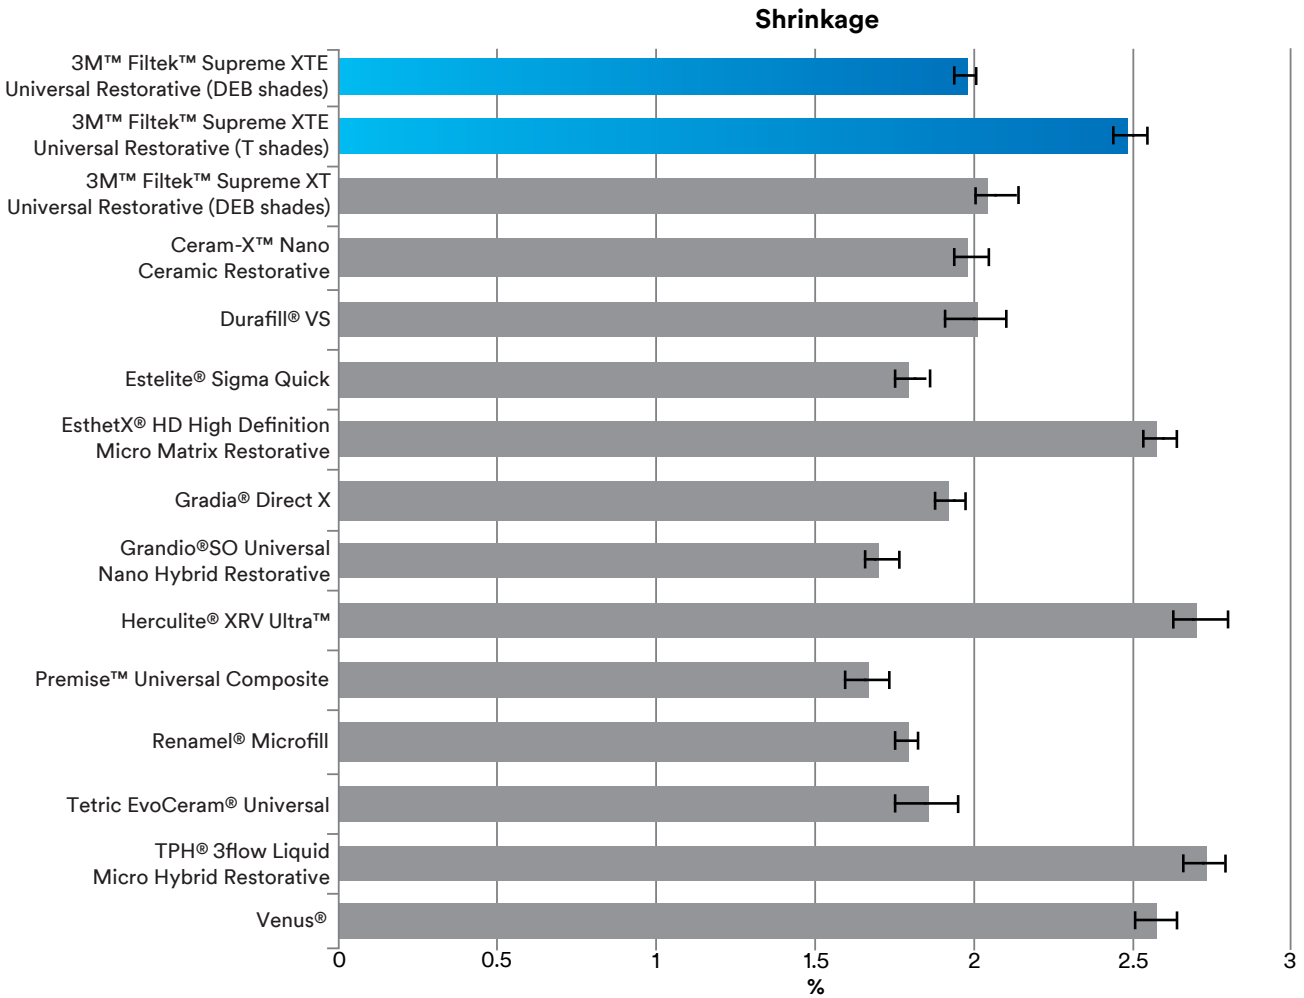

Shrinkage. Source: 3M internal data

The volumetric shrinkage of 3M™ Filtek™ Supreme XTE Universal Restorative DEB shades and T shades is statistically different. The DEB shades of Filtek Supreme XTE restorative are statistically lower than EsthetX® HD High Definition Micro Matrix Restorative, Herculite® XRV Ultra™, TPH® 3flow Liquid Micro Hybrid Restorative and Venus®.


Field Evaluation

A field evaluation was conducted with 256 dentists in three countries (U.S., Germany and Italy) to confirm the *in vitro* handling and assess the aesthetic clinical performance of 3M™ Filtek™ Supreme XTE Universal Restorative. Recruited dentists were sent either capsules or syringes, depending on their delivery preference. In addition, they were screened on their typical composite shade technique. Dentists who were primarily single-shade users in a restoration were sent a selection of the Body shades. Dentists who typically layer multiple shades in a single restoration received a selection of all opacities.


Eighty-three dentists currently use 3M™ Filtek™ Supreme XT Universal Restorative as their most frequently used composite. An additional 74 use it in their practice. One hundred and two were assessed to be primarily single-shade users, and 154 were multi-shade users (in a single restoration).

There were 25,858 placements: 12,606 in anterior restorations and 13,252 in the posterior.


Anterior Single Shade: 8,905

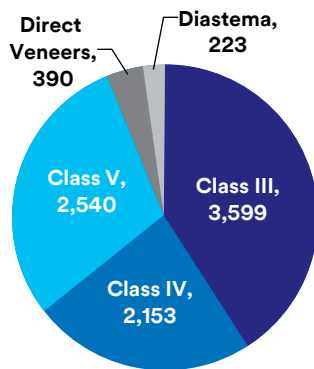


Anterior Multiple Shade: 3,701

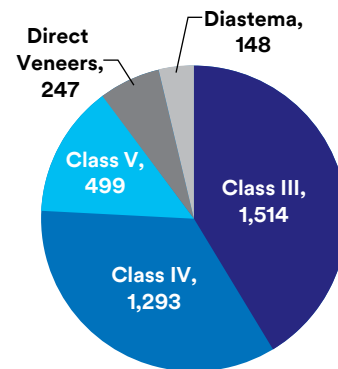

Posterior Single Shade: 11,026

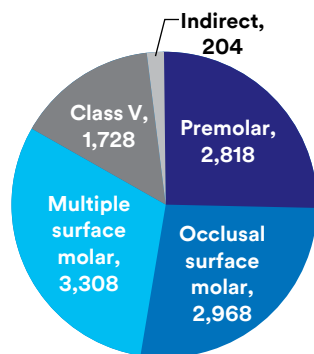

Posterior Multiple Shade: 2,226

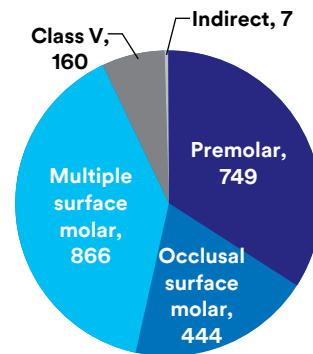


Handling Acceptability

The handling ratings of 3M™ Filtek™ Supreme XTE Universal Restorative were compared to the handling of their most frequently used composite. The data for current 3M™ Filtek™ Supreme XT Universal Restorative users (labeled 3M™ Filtek™ Supreme XT Universal Restorative) was separated from dentists using any other composite more frequently (labeled Competitive Product).


Dentists were asked to rate handling attributes on a 7-point scale. For Viscosity, Stickiness to Instrument, Flow and Ability to Hold Its Shape, a rating of 4 was ideal. For Ease of Shaping and Veneering, Ability to Use a Brush and Cavity/Marginal Adaptation, a rating of 7 was best.

4 is Ideal

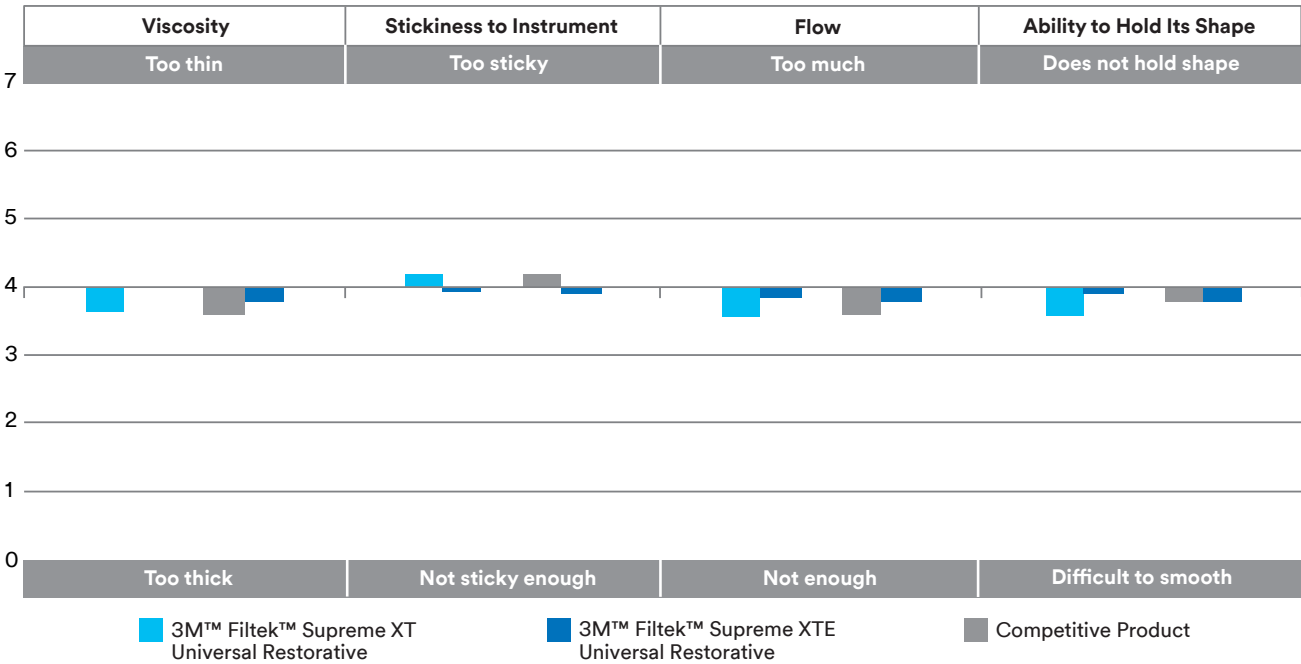

Source: 3M internal data

7 is Best

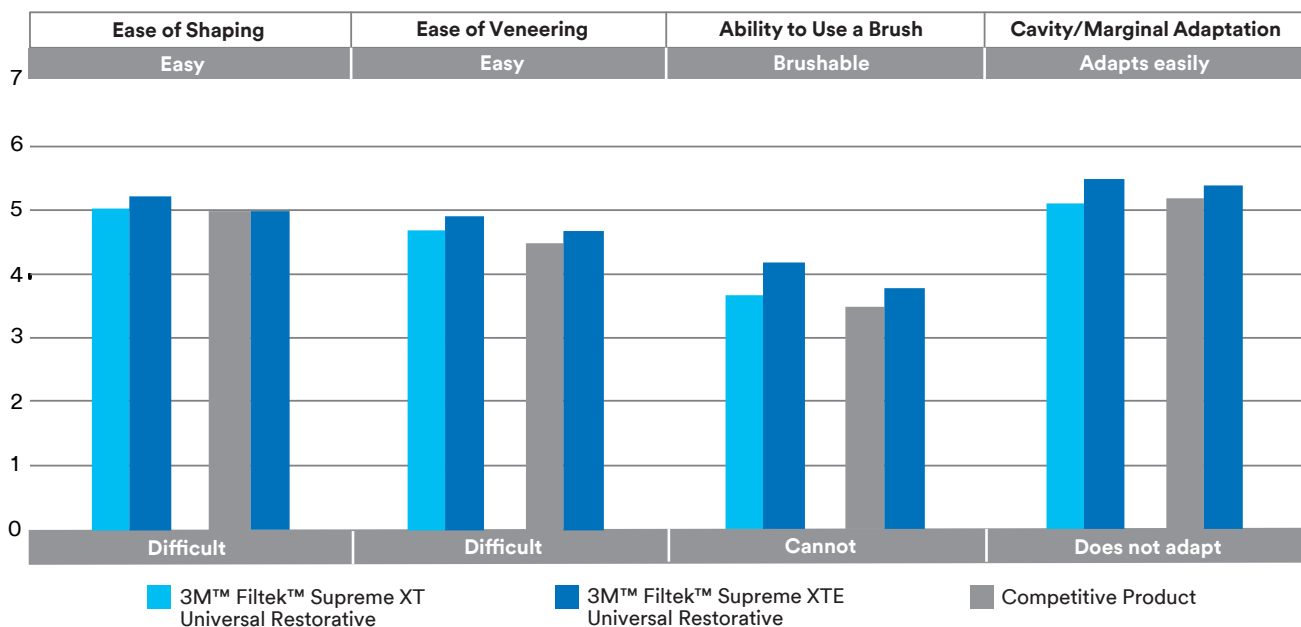


Source: 3M internal data

3M™ Filtek™ Supreme XT Universal Restorative users rated the Viscosity, Stickiness to Instrument, Flow and Ability to Hold Its Shape of 3M™ Filtek™ Supreme XTE Universal Restorative as ideal. In addition, the Viscosity, Stickiness to Instrument, Flow, Ability to Hold Its Shape, and the Ability to Use a Brush was rated statistically higher for Filtek Supreme XTE restorative than their current product.

Competitive product users rated the Stickiness to Instrument of Filtek Supreme XTE restorative as ideal. In addition, the Stickiness to Instrument, Flow and the Ability to Use a Brush were rated statistically higher for Filtek Supreme XTE restorative than their current product.

Dentists were also specifically asked to compare 3M™ Filtek™ Supreme XTE Universal Restorative to their current product on a scale of 1 to 7. A rating of 1–3 indicated Filtek Supreme XTE restorative was Much Worse to Worse than their current product. Ratings of 5–7 indicated Filtek Supreme XTE restorative was Better to Much Better than their current product. A rating of 4 indicated Filtek Supreme XTE restorative was performing similarly to their current product. (For the purpose of this report, the rating of 4 is not shown. It can be calculated by subtracting the Worse and Better % Respondents from 100.)


3M™ Filtek™ Supreme XT Universal Restorative Users

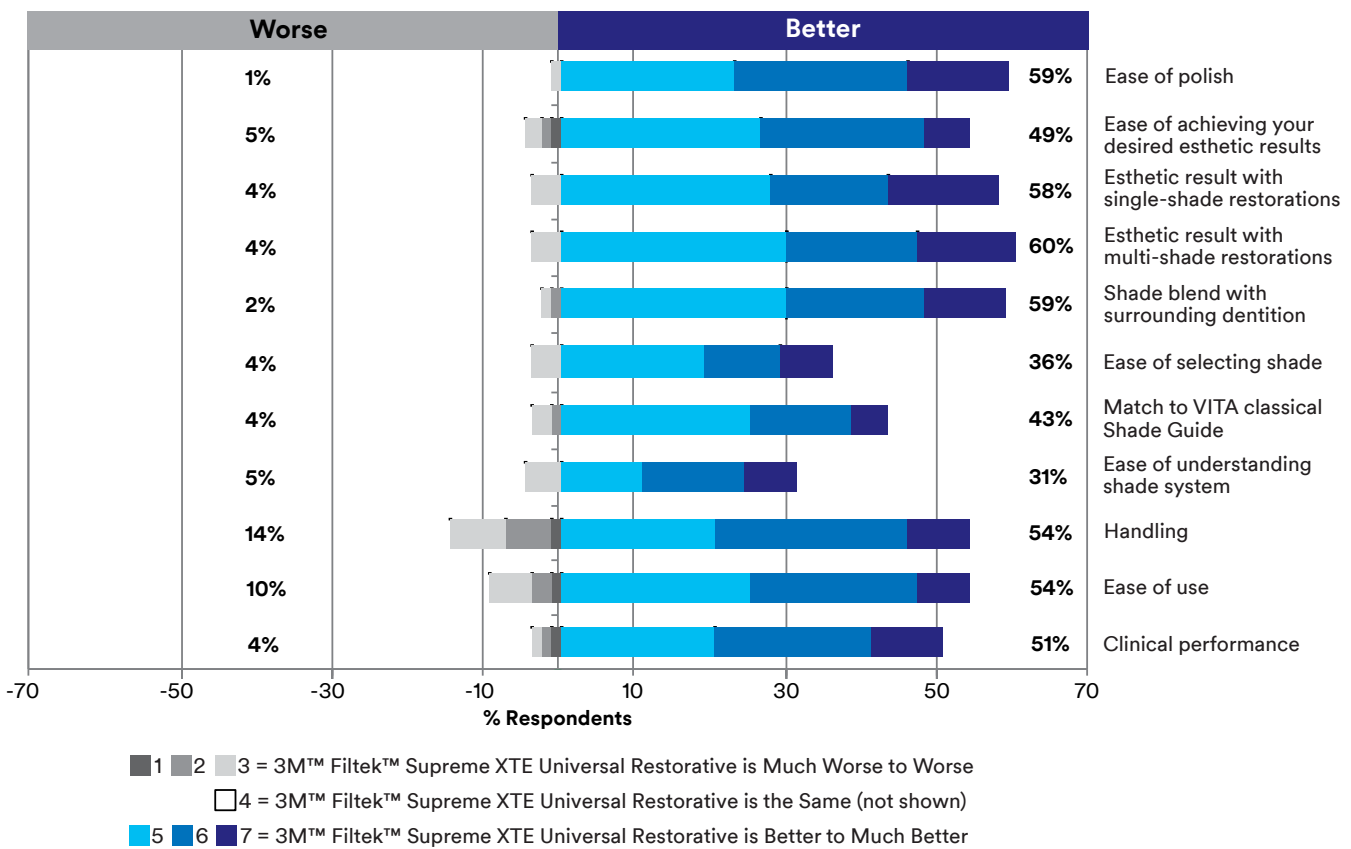

This chart shows the response of the current 3M™ Filtek™ Supreme XT Universal Restorative users. Over 50% of the current Filtek Supreme XT restorative users felt Filtek Supreme XTE restorative exhibited improved:

- Ease of polish
- Results with single- and multi-shade restorations
- Shade blend with surrounding dentition
- Handling
- Ease of use
- Clinical performance

In all aspects except handling, more than 90% of users agreed the performance of Filtek Supreme XTE restorative was the same or better than Filtek Supreme XT restorative. More than 85% rated the handling of Filtek Supreme XTE restorative as the same or better than Filtek Supreme XT restorative.

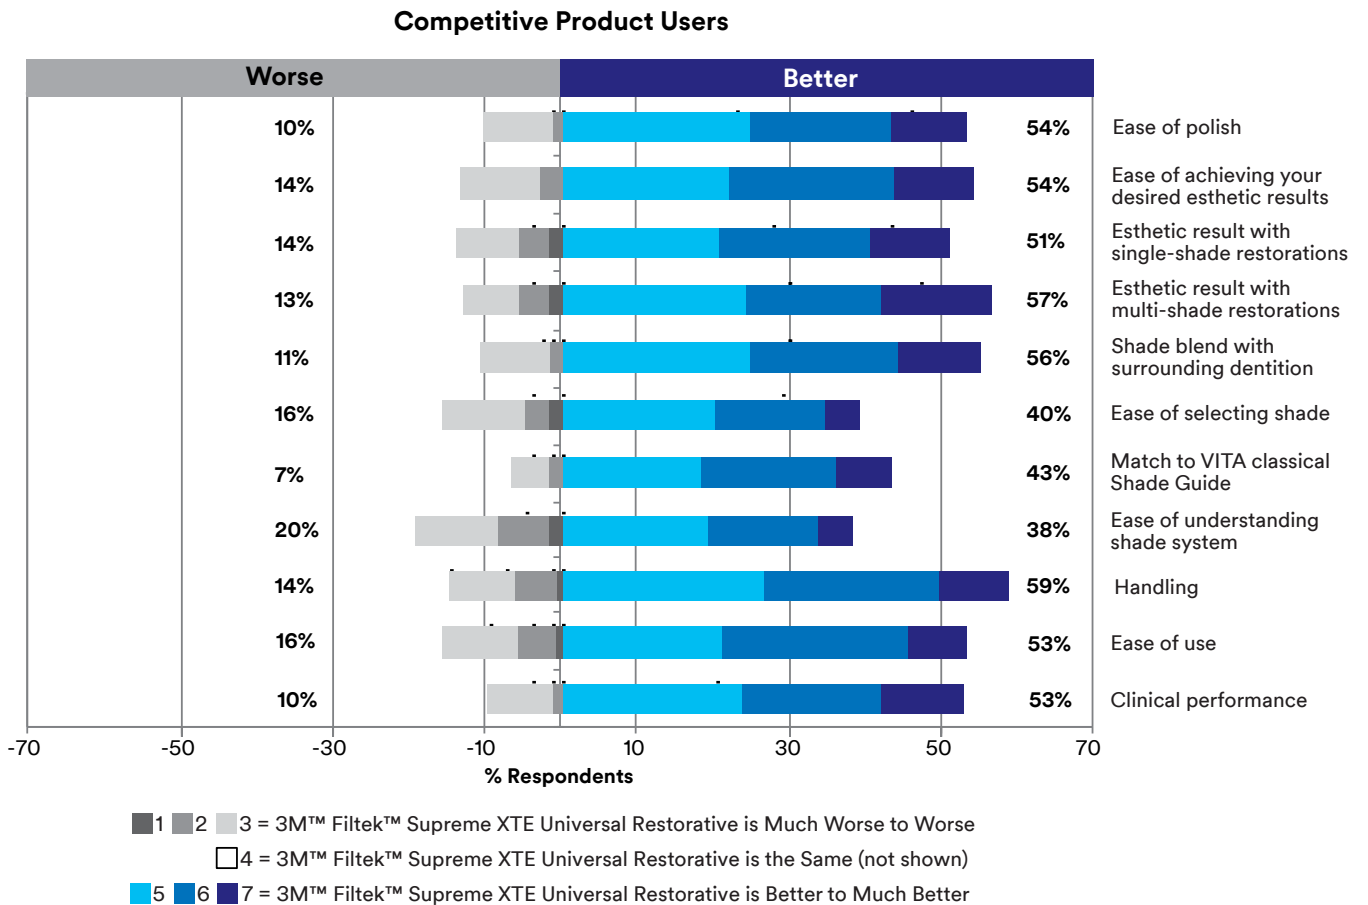

This chart shows the response of the current competitive product users. Over 50% of the current competitive product users felt 3M™ Filtek™ Supreme XTE Universal Restorative exhibited improved:

- Ease of polish
- Ease of achieving your desired aesthetic result
- Results with single- and multi-shade restorations
- Shade blend with surrounding dentition
- Handling
- Ease of use
- Clinical performance

In all aspects except ease of selecting shade, ease of understanding the shade system and ease of use, more than 85% of users agreed the performance of Filtek Supreme XTE restorative was the same or better than their current product. Many of these dentists were not familiar with 3M™ Filtek™ Supreme XT Universal Restorative. Dentists in this study did not receive any shade reference card or shade wheel to assist in shade identification. Even with this handicap, these three attributes were rated the same or better than competitive products by 80% of the dentists.

Questions and Answers

- **This system is too complicated for me. Most of the time I use only one shade in my restorations.**

The 3M™ Filtek™ Supreme XTE Universal Restorative system is designed to be flexible to meet the needs of every dentist. While there are four opacities available, dentists using only one shade in a restoration can use the Body shades. Use of all opacities in this system is not required, but optional.

- **The Translucent shades are very transparent. Tooth structure is not. Where can I use this type of material?**

The Translucent shades can be used either internally or externally in a restoration. These materials can be used to accentuate the recreated Dentine mamelons and maximise translucency of an incisal edge. In addition, they can be used as a very thin layer over the surface of the restoration to take advantage of their excellent polish retention.

- **What is the difference between 3M™ Filtek™ Supreme XT Universal Restorative and Filtek Supreme XTE restorative?**

There have been improvements made in the filler processing and pigments to provide better polish retention, improved fluorescence and Filtek Supreme XT-like handling for all opacities, including translucent.

- **Can I use my old shade wheel (from Filtek Supreme XT restorative) or recipes to create multi-shaded restorations?**

Yes. The colour targets for the shades remain the same. However, due to the modified shade offering, a new wheel (and recipes) was created to take advantage of this enhancement.

Endnotes

1. Mitra, S.B., Wu, D., & Holmes, B.N. (2003). *Journal of the American Dental Association*, 134, 1382–1390.
2. Katholieke Universiteit Leuven clinical study.
3. Dentine, Enamel and Body shades will be referred to as DEB shades throughout this document.
4. Translucent shades will be referred to as T shades throughout this document.
5. Takahashi, M.K., Viera, S., Rached, R.N., Almeida, J.B., Aguiar, M., & Souza, E.M. (2008). *Operative Dentistry*, 33(2), 189–195.
6. Kobussen, G.A., Craig, B.D., Halvorson, R.H., Doruff, M.C., & Bigham, W.S. (2009). Optical Properties of Highly Aesthetic Composite Restoratives, *Journal of Dental Research*, 88(Spec Iss A), 1508.
7. Lee, Y.K. (2005). Measurement of Opalescence of Resin Composites. *Dental Materials*, 21, 1068–1074.
8. Kobussen, G.A.
9. Dr. Jorge Perdigao, University of Minnesota, Division of Operative Dentistry, Department of Restorative Science.
10. Uncured paste was dissolved in acetone and then centrifuged. The supernatant liquid was removed and the residue dissolved in acetone, then centrifuged.
11. AFM—Atomic Force Microscopy in a 3D surface plot. Scanned area is about 100um². The Tapping Mode AFM uses a single crystal silica probe with a force constant of ~40N/m to determine the surface profile. The darker the colour, the deeper the gouge; the lighter the colour, the higher the peak (the pink colour indicates the maximum instrument capability).
12. Ibid
13. Ibid
14. Ra is the arithmetic average of the absolute values of the surface height deviations from the mean surface plane calculated from the 500×500μ² Wyko maps.
15. Watts, D.C., & Cash, A.J. (1991). *Measurement Science and Technology*, 2, 788–794.

Technical Data Summary

	Level	3M™ Filtek™ Supreme XTE Universal Restorative (DEB shades)	3M™ Filtek™ Supreme XTE Universal Restorative (T shades)	3M™ Filtek™ Supreme XT Universal Restorative (DEB shades)	Ceram-X™ Nano Ceramic Restorative	Durafill® VS
Compressive Strength	MPa	370.56	394.01	361.37	346.80	349.86
	StDev	15.13	25.05	23.78	22.96	10.40
Diametral Tensile Strength	MPa	86.12	90.64	85.53	63.31	55.89
	StDev	3.91	1.40	5.47	6.49	2.87
Flexural Strength	MPa	165.14	157.98	165.90	113.68	64.50
	StDev	13.59	8.16	5.40	11.52	3.62
Flexural Modulus	MPa	11,348.00	9,180.00	11,436.00	8,830.00	2,613.00
	StDev	271.00	431.00	442.00	379.00	66.00
Fracture Toughness	K1c	1.84	1.51	1.92	1.69	1.01
	StDev	0.19	0.03	0.21	0.05	0.09
Shrinkage	%	1.97	2.48	2.06	1.97	2.00
	StDev	0.03	0.06	0.06	0.05	0.08
Polish Retention						
Initial	Mean	94.83	93.83	92.81	72.90	86.33
	StDev	1.03	1.39	2.35	—	0.15
500 cycles	Mean	86.82	88.04	83.09	36.03	74.82
	StDev	5.77	6.01	6.08	7.27	4.85
1,000 cycles	Mean	83.32	85.72	78.73	25.50	68.08
	StDev	5.96	5.60	7.69	6.39	5.67
2,000 cycles	Mean	76.55	82.83	69.74	23.18	59.03
	StDev	6.43	5.12	8.57	2.74	6.15
3,000 cycles	Mean	73.19	82.01	62.89	10.45	58.70
	StDev	5.99	5.96	8.69	1.37	3.38
4,000 cycles	Mean	70.33	81.23	56.63	9.80	55.67
	StDev	5.52	4.15	7.28	1.23	6.57
5,000 cycles	Mean	69.66	79.80	53.48	9.55	54.02
	StDev	5.36	6.05	8.19	1.00	3.57
6,000 cycles	Mean	68.62	79.72	54.73	7.98	53.21
	StDev	4.77	4.42	7.75	0.71	6.32
3-Body Wear Rate	um lost	5.61	6.54	5.07	32.04	15.22
	StDev	0.63	0.50	0.80	0.68	0.55

	Level	Estelite® Sigma Quick	EsthetX® HD High Definition Micro Matrix Restorative	Gradia® Direct X	Grandio®SO Universal Nano Hybrid Restorative	Herculite® XRV Ultra™	Premise™ Universal Composite
Compressive Strength	MPa StDev	364.19 14.03	376.83 35.41	323.40 7.92	341.84 16.04	349.10 23.51	370.81 18.83
Diametral Tensile Strength	MPa StDev	77.56 2.98	73.64 2.38	52.82 5.89	81.28 5.63	80.65 5.76	65.89 8.18
Flexural Strength	MPa StDev	111.08 3.94	132.90 8.65	106.07 6.77	144.03 17.54	106.48 14.34	108.64 9.64
Flexural Modulus	MPa StDev	7,552.00 202.00	10,128.00 146.00	6,299.00 185.00	19,437.00 299.00	7,679.00 541.00	7,839.00 183.00
Fracture Toughness	K1c StDev	— —	1.70 0.12	1.05 0.06	1.68 0.07	— —	1.81 0.03
Shrinkage	% StDev	1.80 0.05	2.58 0.05	1.92 0.04	1.69 0.04	2.70 0.07	1.66 0.06
Polish Retention							
Initial	Mean StDev	93.93 0.68	92.45 2.33	76.17 0.32	67.27 1.71	89.67 2.17	91.60 0.96
500 cycles	Mean StDev	67.62 7.45	54.75 3.86	37.98 10.27	43.47 4.82	69.63 9.21	70.36 5.97
1,000 cycles	Mean StDev	64.14 3.75	27.65 1.03	21.58 12.86	35.31 6.34	60.83 7.29	63.11 5.81
2,000 cycles	Mean StDev	63.55 3.88	25.05 2.64	13.53 5.00	20.79 3.29	54.89 6.85	49.35 8.48
3,000 cycles	Mean StDev	64.29 9.89	29.28 2.59	13.00 0.81	17.26 2.81	52.57 11.34	44.12 4.93
4,000 cycles	Mean StDev	62.35 3.66	26.78 6.12	10.47 0.89	13.13 1.33	53.71 5.48	39.29 6.97
5,000 cycles	Mean StDev	63.30 9.53	28.68 0.65	11.77 1.16	12.16 0.96	52.84 11.58	39.26 3.12
6,000 cycles	Mean StDev	65.01 3.33	27.65 1.01	10.55 1.22	11.48 0.98	54.88 4.57	37.18 5.00
3-Body Wear Rate	um lost StDev	7.50 0.46	7.38 0.31	15.17 1.43	8.49 0.64	15.78 2.13	16.27 0.55

3M.com.au/Filtek
3M.co.nz/Filtek



3M Oral Care

3M Australia Pty Limited
Building A, 1 Rivett Rd
North Ryde NSW 2113
Ph: 1300 363 454
www.3M.com.au

3M New Zealand Limited
94 Apollo Drive
Rosedale Auckland 0632
Ph: 0800 80 81 82
www.3M.co.nz



Find us on Facebook

Please always refer to the 3M Product Instructions For Use. 3M, ESPE, Filtek and Visilux are trademarks of 3M. All other trademarks are not trademarks of 3M. © 3M 2018. All rights reserved.